

Journal of Clinical Chemistry and Clinical Biochemistry

Zeitschrift für Klinische Chemie und Klinische Biochemie

Gemeinsames Organ der Deutschen, der Niederländischen, der Österreichischen und der Schweizerischen Gesellschaft für Klinische Chemie

Editors in Chief Verantwortliche Herausgeber

Johannes Büttner, Hannover Ernst Schütte, Berlin

Managing Editor Schriftleiter Friedrich Körber, Berlin

Co-ordinator for IFCC Recommendations Nils-Erik Saris, Helsinki

Editors Herausgeber

Johannes Büttner, Hannover
Jörg Frei, Lausanne
Wolfgang Gerok, Freiburg
Helmut Greiling, Aachen
Walter Guder, München
Erich Kaiser, Wien

Esso Johannes van Kampen, Groningen
Hermann Mattenheimer, Chicago
Ernst Schütte, Berlin
Dankwart Stamm, München
Hansjürgen Staudinger, Freiburg
Otto Wieland, München

Advisory Board unter Mitarbeit von

Klaus Borner, Berlin
Eckhart Buddecke, Münster
Hans-Christoph Curtius, Zürich
Manfred Doss, Marburg
Hartmut Dost, Gießen
Hans Faillard, Saarbrücken
Günther Fuchs, Berlin
Erich Gladtke, Köln
Heinz-Werner Goedde, Hamburg
Erwin Hansert, München

Hans Ludwig Kruskemper, Düsseldorf
Georg Löffler, Regensburg
Mathias M. Müller, Wien
Kurt Oette, Köln
Jean-Paul Persijn, Amsterdam
Ladislaus Róka, Gießen
Ellen Schmidt, Hannover
Ivar Trautschold †, Hannover
Gerhard Uhlenbrück, Köln

Volume 22, 1984



Walter de Gruyter · Berlin · New York

Contents/Inhaltsübersicht

Reviews/Übersicht

- Knoll, E. and Wisser, H.
Problems in the development of radioimmunoassay of catecholamines
Probleme bei der Entwicklung eines Radioimmunoassay für Katecholamine
741

Original papers/Originalarbeiten

- Agabiti-Rosei, E., Beschi, M., Castellano, M., Tosoni, S. and Signorini, C.
Plasma catecholamines assay:
Comparison between fluorimetric and radioenzymatic method
Bestimmung der Catecholamine im Plasma:
Vergleich zwischen fluorimetrischer und radioenzymatischer Methode 539
- Allner, R.
Rheumafaktoren und Immunglobuline als Störquellen bei einem heterogenen Enzym-Immunoassay
Rheumatoid factors and immunoglobulins as interfering factors in an heterogeneous enzyme immunoassay 759
- Amodio, P., Gatta, A. and Ruol, A.
 β_2 -Microglobulin concentration in plasma and production in liver cirrhosis
Konzentration von β_2 -Mikroglobulin im Plasma und Bildung bei Lebercirrhose 147
- Assink, H. A., Blijenberg, B. G., Boerma, G. J. M. and Leijnse, B.
The introduction of bromocresol purple for the determination of serum albumin on SMAC and ACA, and the standardization procedure
Die Einführung von Bromkresolpurpur für die Bestimmung von Albumin im Serum mit dem SMAC und dem ACA sowie das Standardisierungsverfahren 685
- Assmann, G., Jabs, H.-U., Nolte, W. and Schriewer, H.
Precipitation of LDL with sulphopolyanions:
A comparison of two methods for LDL cholesterol determination
Präzipitation von LDL mit Sulfopolyanionen:
Vergleich zweier Methoden zur LDL-Cholesterin-Bestimmung 781
- Assmann, G., Menzel, H. J., Kladetzky, R. G. and Büttner, G.
Frequency of apolipoprotein A-I mutants in the German population
Zur Häufigkeit von Apolipoprotein A-I-Mutanten in der deutschen Bevölkerung 585
- Assmann, G., Schulte, H. and Schriewer, H.
The effects of cigarette smoking on serum levels of HDL cholesterol and HDL apolipoprotein A-I
Findings of a prospective epidemiological study on employees of several companies in Westphalia, West Germany
Einfluß des Zigarettenrauchens auf die Konzentration von HDL-Cholesterin und HDL-Apolipoprotein A-I im Bluts serum
Ergebnisse der prospektiven epidemiologischen Studie bei Betriebsangehörigen in Westfalen 397
- Balcke, P., Schmidt, P., Zazgornik, J., Haubenstock, A. and Kopsa, H.
In vitro synthesis of oxalic acid has no relevant influence on plasma oxalic acid levels in haemodialysis patients
In vitro-Synthese von Oxalsäure ist ohne Bedeutung für die Bestimmung von Oxalsäure im Plasma bei Hämodialysepatienten 261
- Becker, J. U.
Bestimmung der Konzentration eines neuen Antiarrhythmicums, Flecainid, im Plasma durch Hochleistungsflüssigkeitschromatographie (HPLC): Probenvorbereitung durch Extraktionssäulen
Measurement of the plasma concentration of a new antiarrhythmic agent, flecainid, using high performance liquid chromatography (HPLC) and sample preparation with extraction columns 389
- Biber, A. and Hempel, K.
Radioimmunoassay of oxidized calmodulin in chloramine-T treated tissue samples
Radioimmunologische Bestimmung von oxidiertem Calmodulin in Chloramin-T behandelten Proben 185
- Blijenberg, B. G., Brouwer, H. J., Roetering, H. A. and Leijnse, B.
Surveys of neonatal bilirubin. An evaluation
Auswertung von Ringversuchen für die Bilirubinbestimmung bei Neugeborenen 609
- Bollinger, F., Mahler, A., Clinet, G. and Delmotte, P.
Measles antibodies, anti-proteinase and plasminogen distribution in serum and plasma from patients affected with multiple sclerosis and patients affected with non-neurological diseases
Masern-Antikörper-, Proteaseinhibitoren- und Plasminogen-Verteilung in Serum und Plasma bei Patienten mit Multipler Sklerose und nicht-neurologischen Erkrankungen 653
- Bosch, Anneke M. G.
A radio-immunoassay of 19-nortestosterone using celite column chromatography
Radioimmunoassay von 19-Nortestosteron nach Säulenchromatographie an Celit 29
- Bossmann, Bärbel und Haschen, R. J.
De novo synthesis of brush border membrane enzymes during intestinal perfusion with bile salt in the rat
De novo-Synthese von Enzymen der Bürstensaummembran der Ratte während Perfusion des Darms mit Gallensalz 449
- Brechbühler, T., Kaeslin, M. and Wyler, F.
Reference values of various blood constituents in young minipigs
Referenzwerte verschiedener Blutbestandteile beim jungen Miniatschwein 301
- Breuer, N., Dommes, P., Tandon, R. und Goebell, H.
Isolierung und Quantifizierung nicht-sulfatiertes und sulfatiertes Gallensäuren im Stuhl
Isolation and quantification of non-sulphated and sulphated bile acids in faeces 623
- Bruchelt, G. and Schmidt, K. H.
Comparative studies on the oxidative processes during phagocytosis measured by luminol-dependent chemiluminescence
Vergleichende Untersuchungen von oxidativen Prozessen während der Phagozytose mittels Luminol-abhängiger Chemilumineszenz 1

Costongs, G. M. P. J., Janson, P. C. W. and Brombacher, P. J.	
Effects of biological and analytical variations on the appropriate use of "reference intervals" in Clinical Chemistry	
Proposal of a scheme for longitudinal assessment of laboratory values	
Wirkungen biologischer und analytischer Varianzen auf den angemessenen Gebrauch von „Referenzintervallen“ in der Klinischen Chemie.	
Vorschlag eines Schemas zur longitudinalen Bewertung von Laboratoriumsergebnissen	613
Dörner, K., Campos, R. and Börnsen, Susanne	
Further evaluation of the SG test strip for estimation of urinary osmolality	
Weitergehende Untersuchungen zur Abschätzung der Urin-Osmolalität mit dem SG-Teststreifen	419
Dresow, B. and Delbrück, A.	
The isolation and activity of growth-stimulating factors from human platelets	
Zur Isolierung und Wirkung von wachstumsstimulierenden Faktoren aus menschlichen Thrombocyten	527
Falk, U., Schmidt-Gayk, H. and Hüfner, M.	
Radioimmunoassay for serum thyroglobulin designed for early detection of metastases and recurrences in the follow-up of patients with differentiated thyroid carcinoma	
Radioimmunoassay für Thyreoglobulin im Serum zur Früherkennung von Rezidiven und Metastasen in der Nachsorge von Patienten mit differenzierten Schilddrüsenkarzinomen	661
Fogh-Andersen, N., Ladefoged, J. and Møller-Petersen, J.	
Renal and hepatic extraction of carboxyl-terminal immunoreactive parathyroid hormone in normal man	
Renale und hepatische Extraktion von carboxyterminalem immunreaktiven Parathyroidhormon bei Gesunden	479
Gadow, A., Fricke, H., Strasburger, C. J. and Wood, W. G.	
Synthesis and evaluation of luminescent tracers and haptens-protein conjugates for use in luminescence immunoassays with immobilised antibodies and antigens	
A critical study of macro solid phases for use in immunoassay systems Part II Synthese und Beurteilung von Lumineszenz-Markern und Haptens-Protein-Konjugaten für Lumineszenz-Immunoassays mit immobilisierten Antikörpern und Antigenen	
Eine kritische Untersuchung von Makro-Festphasen zum Gebrauch in Immunoassay-Systemen, Teil II	337
Gardiner, P. E., Gessner, H., Brägger, P., Stoeppler, M. and Nürnberg, H. W.	
The distribution of zinc in human erythrocytes	
Die Verteilung von Zink in menschlichen Erythrozyten	159
Garth, H. und Zoch, E.	
Kontinuierliche Messung der katalytischen Aktivität von Adenosindesaminase mit der pH-Stat-Methode	
The continuous measurement of adenosine deaminase activity by the pH-stat-method	769
Golf, S. W. and Graef, V.	
Rat liver 3-oxo-5α-steroid Δ ⁴ -dehydrogenase. Modulation of enzyme activity by changes in phosphorylation state	
Modulation der Enzymaktivität der 3-Oxo-5α-steroid Δ ⁴ -Dehydrogenase aus der Rattenleber durch Veränderung des Phosphorylierungszustandes	705
Golf, S. W., Happel, O., Graef, V. and Seim, K. E.	
Plasma aldosterone, cortisol and electrolyte concentrations in physical exercise after magnesium supplementation	
Aldosteron-, Cortisol- und Elektrolytkonzentrationen im Plasma bei körperlicher Belastung unter Magnesiumsubstitution	717
Golf, S. W., Kaul-Kunz, C. and Róka, L.	
Creatine kinase isoenzyme MB determination on the ACA: Dependence on serum matrix and other effectors	
Bestimmung der katalytischen Aktivität von Kreatinkinase Isoenzym MB mit dem ACA:	
Abhängigkeit von der Serummatrix und anderen Effektoren	751
Golf, S. W., Temme, H., Kempf, K. D., Bleyl, H., Brüstle, A., Bödeker, R. and Heinrich, D.	
Systemic short-term fibrinolysis with high-dose streptokinase in acute myocardial infarction: Time course of biochemical parameters	
Systemische Kurzzeitlyse mit hochdosierter Streptokinase bei Patienten mit akutem Myokardinfarkt: Verlauf der biochemischen Kenngrößen	723
Gressner, A. M.	
Aminoterminal propeptides of type III procollagen in human cerebrospinal fluid	
Aminoterminale Propeptide von Typ III Prokollagen im Liquor cerebrospinalis des Menschen	237
Gressner, A. M. and Peltzer, Birgit	
Amidolytic and immuno-nephelometric determination of α ₁ -proteinase inhibitor and α ₂ -macroglobulin in serum with calculation of specific inhibitor activities in health and disease	
Amidolytische und immun-nephelometrische Bestimmung von α ₁ -Proteinase Inhibitor und α ₂ -Makroglobulin im Serum mit Berechnung der spezifischen inhibitorischen Aktivitäten bei Gesunden und Kranken	633
Gruhl, H. und Mayer, H.	
Einfache und rasche Bestimmung von Thiopental im Serum mit HPLC	
A simple and rapid determination of serum thiopental by HPLC	385
Guder, W. G., Fürschel, Susanne, Vandewalle, A. and Wirthensohn, Gabriele	
Bioluminescence procedures for the measurement of NAD(P) dependent enzyme catalytic activities in submicrogram quantities of rabbit and human nephron structures	
Biolumineszenzverfahren zur Messung NAD(P)abhängiger Enzymaktivitäten in einzelnen Nephronstrukturen der Kaninchen und Menschen	129
Günther, T., Vormann, J. and Merker, H. J.	
Effect of magnesium injection on foetal development	
Wirkung von Magnesium-Injektionen auf die Foetalentwicklung	473
Hagemeier, E., Kemper, K., Boos, K.-S. and Schlimme, E.	
Development of a chromatographic method for the quantitative determination of minor ribonucleosides in physiological fluids	
Characterization and quantitative determination of minor ribonucleosides in physiological fluids, Part I	
Entwicklung einer chromatographischen Methode zur quantitativen Bestimmung seltener Ribonucleoside in physiologischen Flüssigkeiten	
Charakterisierung und quantitative Bestimmung von seltenen Ribonucleosiden in physiologischen Flüssigkeiten, Teil I	175
Hansert, E., Federkiel, H. and Stamm, D.	
A new procedure for discriminating between two patient populations using multivariate decision limits:	
Application in the detection and exclusion of alcoholism based on clinical laboratory findings	
Neues Verfahren zur Diskrimination zweier Patientenstichproben unter Verwendung multivariater Entscheidungsgrenzen:	
Anwendung zur Erkennung und zum Ausschluß des Alkoholismus aufgrund klinisch-chemischer Befunde	791
Heinemann, G., Schievelbein, H. und Richter, Fridrun	
Die analytische und diagnostische Validität der Bestimmung von Carboxyhaemoglobin im Blut und Kohlenmonoxid in der Atemluft von Rauchern und Nichtrauchern	
Analytic and diagnostic validity of the determination of carboxyhaemoglobin in blood, and carbon monoxide in breath of smokers and non-smokers	229
Henkel, E., Morich, Susanne and Henkel, Renate	
2-Chloro-4-nitrophenyl-β-D-maltoheptaoside:	
A new substrate for the determination of α-amylase in serum and urine	
2-Chloro-4-nitrophenyl-β-D-maltoheptaosid:	
Ein neues Substrat zur Bestimmung von α-Amylase in Serum und Harn	489

Hijikata, Yasuyo, Hara, Katsuko, Shiozaki, Yasuko, Murata, Kenjiro and Sameshima, Yoshiko	Multicentre study of a new enzymatic method of cholesterol determination Multizentrische Erprobung einer neuen enzymatischen Cholesterinbestimmung	Külpmann, W. R., Gey, S., Beneking, M., Kohl, B. and Oellerich, M.	
Determination of free tryptophan in plasma and its clinical applications Bestimmung des freien Tryptophan im Plasma und ihre klinische Anwendung	245	Determination of total and free phenytoin in serum by non-isotopic immunoassays and gas chromatography Bestimmung von Gesamt- und freiem Phenytoin im Serum mit radioaktivitätsfreien Immunoassays und Gaschromatographie	773
Höfeler, H. and Klingemann, H.-G.		Lapin, A., Endler, A. T., Ogunyemi, E. O. and Gabl, F.	
Fibronectin and factor VIII-related antigen in liver cirrhosis and acute liver failure		Two dimensional electrophoresis method for additional characterization of paraproteins in serum	
Fibronectin und Faktor VIII-assoziiertes Antigen bei Lebercirrhose und akutem Leberversagen	15	Clinical application of two dimensional electrophoresis, I	
Hutt, V., Klör, H. U., Wechsler, J. G. und Ditschuneit, H.	The measurement of androst-4-en-17β-ol-3,11-dione (11-oxotestosterone) by radioimmunoassay in human plasma Radioimmunoassay zur Messung von Androst-4-en-17β-ol-3,11-dion (11-Oxotestosteron) im Plasma des Menschen	Zweidimensionale Elektrophorese-Methode für eine zusätzliche Charakterisierung von Paraproteinen	
Zusammensetzung der Lipoproteinfaktionen VLDL, LDL und HDL bei Hyperlipämikern der Typen IIa, IIb, III, IV und V im Vergleich zu Stoffwechselgesunden	461	Klinische Anwendung von zweidimensionaler Elektrophorese, I	53
Composition of VLDL, LDL and HDL lipoprotein fractions in type IIa, IIb, III, IV and V hyperlipaemic patients and in normal individuals	141		
Javeri, Shailaja and Uhlenbrück, G.		Lindena, J., Büttner, D. and Trautschold, I.	
Isolation of a β-galactosidase from chicken liver		Biological, analytical and experimental components of variance in a long-term study of plasma constituents in rat	
Isolierung einer β-Galaktosidase aus Hühnerleber	735	Biologische, analytische und experimentelle Varianzkomponenten von Plasmarkmalen in einer Langzeitstudie bei der Ratte	97
Jelić, Z., Majkić-Singh, N., Spasić, S., Todorović, P. and Živanov-Stakić, D.		Lizana, J. and Olsson, I.	
Effects of analgesic and antirheumatic drugs on the assay of serum enzymes		High resolution isoelectric focusing in a narrow pH interval for the phenotyping of vitamin D-binding protein (Gc-globulin)	
Einfluß analgetischer und antirheumatischer Medikamente auf die Bestimmung von Enzymen im Serum	559	Hochauflösende isoelektrische Fokussierung in einem engen pH-Bereich zur Phänotypisierung des Vitamin D bindenden Proteins (Gc-Globulin)	
Jung, K., Pergande, Monika, Reinholdt, Carmen, Schulze, B., Scholz, D. and Strobel, V.	Kossmann, K. T.	545	
Multiple forms of alanine aminopeptidase, alkaline phosphatase and γ-glutamyltransferase in urine of healthy persons, patients suffering from kidney diseases and patients with kidney transplants	Hochauflösende zweidimensionale Gel-elektrophorese: Eine Methode für das klinisch-chemische Laboratorium High resolution two dimensional gel electrophoresis: A method for the clinical chemistry laboratory		
Multiple Formen der Alaninaminopeptidase, alkalischen Phosphatase und γ-Glutamyltransferase im Urin von gesunden Personen, Patienten mit Nierenerkrankungen und nierentransplantierten Patienten	253		
Juretić, Dubravka, Lipovac, K., Hadžija, M. and Slijepčević, M.	Knoll, E., Müller, F. W., Ratge, D., Bauersfeld, W. and Wisser, H.	Manz, B., Rehder, Marianne, Heubner, A., Kreienberg, R., Grill, H.-J. and Pollow, K.	
Effect of the degree of hyperglycaemia on the catalytic activities of glycosidases in kidney and urine of diabetic rats	Influence of food intake on concentrations of plasma catecholamines and cortisol	17β-Carboxamide steroids: Highly effective inhibitors of the phytohaemagglutinin mediated blastogenesis of normal human peripheral lymphocytes	
Einfluß des Hyperglykämie-Grades auf die katalytischen Aktivitäten von Glykosidasen in Nieren und Harn diabetischer Ratten	Einfluß der Nahrungsaufnahme auf die Konzentrationen von Katecholaminen und Cortisol im Plasma	17β-Carboxamid-Steroide: Hochwirksame Inhibitoren der phytohämaggulatin-induzierten Blastogenese normaler peripherer menschlicher Lymphocyten	
Kattermann, R., Jaworek, D. and Möller, G. in collaboration with Assmann, G., Björkhem, I., Svensson, L., Borner, K., Boerma, G., Leijnse, B., Desager, J. P., Harwengt, C., Kupke, Irene and Trinder, P.	Knüppel, W., Neumeier, D., Fateh-Moghadam, A. und Knedel, M.	209	
	Rechnerunterstützte Befundung von Eiweißelektrophoresen auf Celluloseacetatfolie Computer assisted interpretative reporting for serum protein electrophoresis on cellulose acetate film	Marwaha, R. K. and Johnson, B. F.	
	407	A radioimmunoassay for digoxin in human urine Radioimmunoassay für Digoxin im Harn des Menschen	
	Kreuzfelder, E., Kuwert, E., Windeck, R., Graben, N., Pistor, K. und Heber, F.	403	
	Radioimmuntest zur Bestimmung von Humanmyoglobin: Untere Nachweisgrenze, Präzision, Verlaufskontrolle beim myoglobinurischen Nierenversagen	Masson, P. and Hultberg, B.	
	A radioimmunoassay for human myoglobin:	Action pattern of serum amylase using <i>p</i> -nitrophenyl-maltoheptaoside as substrate	
	Lower detection limit, precision, and use in following the course of myoglobinuric kidney failure	Wirkungs-Muster von Amylase im Serum bei Anwendung von <i>p</i> -Nitrophenyl-maltoheptaosid als Substrat	
	61	427	
		Matsumoto, Akira and Fujita, Takuo	
		Abnormalities in erythrocyte membrane protein in pseudohypoparathyroidism type 1	
		Abweichungen im Proteinspektrum der Erythrocytenmembran bei Pseudohypoparathyreoidismus Typ 1	
		281	

Mössner, Ellen, Pfeiderer, G. and Dittel, K. D.	Vergleich verschiedener Regressionsverfahren für Methodenvergleichsstudien und Bestimmung von Stichprobenumfängen	Schädlich, H.-J., Bliersbach, Y., Felgenhauer, K. und Schifferdecker, M.
Placental alkaline phosphatase in tumour tissue and serum	Methodenvergleichsstudien in der Klinischen Chemie, Teil II	Immunglobulin G synthetisierende Lymphocyten im Liquor bei Multipler Sklerose und nichtentzündlichen Erkrankungen des Nervensystems
Placentare alkalische Phosphatase in Tumorgewebe und Serum	467	Occurrence of immunoglobulin G-synthesizing lymphocytes in cerebrospinal fluid in multiple sclerosis and non-inflammatory diseases of the nervous system
Nägele, U., Hägele, E. O., Sauer, G., Wiedemann, E., Lehmann, P., Wahlefeld, A. W. and Gruber, W.	Ratnaike, R. N., Butterly, J. E. and Hoffmann, Sheryl	Schleicher, E. and Wieland, O. H.
Reagent for the enzymatic determination of serum total triglycerides with improved lipolytic efficiency	Blood ammonia measurement using a simple reflectometer	Changes of human glomerular basement membrane in diabetes mellitus
Reagenz zur enzymatischen Bestimmung von Triglyceriden im Serum mit verbesselter lipolytischer Wirksamkeit	Bestimmung von Ammoniak im Blut mit einem einfachen Reflektometer	Änderungen der menschlichen glomerulären Basalmembran bei Diabetes mellitus
165		223
Neuhäuser, M., Göttmann, U. und Bäßler, K. H.	Rehpenning, W., Harm, K., Ringe, J.-D., Bützow, G. H. und Voigt, K. D.	Scholer, A. and Hohenwallner, W.
Über den Einfluß der Nahrungs zusammensetzung auf die Ausscheidung von 3-Methylhistidin und Kreatinin im Harn	Quasi-verteilungsfreie multivariate Beurteilung klinisch-chemischer Kenngrößen mit Hilfe der X-Transformation von <i>van der Waerden</i>	Evaluation of a colorimetric test for the determination of α -amylase with <i>p</i> -nitrophenylheptaoside as substrate
Dietary effects on the urinary excretion of 3-methylhistidine and creatinine	Quasi-distribution-free multivariate assessment of patients' data with the aid of the X-transformation of <i>van der Waerden</i>	Evaluierung eines kontinuierlichen Farbtests zur Bestimmung von α -Amylase mit <i>p</i> -Nitrophenylmaltoheptaosid als Substrat
731	319	677
Neumann, S., Gunzer, G., Henrich, N. and Lang, H.	Rick, W. und Hockeborn, M.	Schriewer, H., Assmann, G., Sandkamp, M. und Schulte, H.
“PMN-elastase assay”:	Katalytische Aktivität der Serumlipase im kontinuierlichen titrimetrischen Test in Abhängigkeit von der Temperatur	The relationship of lipoprotein (a) (<i>Lp(a)</i>) to risk factors of coronary heart disease:
Enzym immunoassay for human polymorphonuclear elastase complexed with α_1 -proteinase inhibitor	The effect of temperature on the catalytic activity of serum lipase in the continuous titrimetric assay	Initial results of the prospective epidemiological study on company employees in Westfalia
“PMN-Elastase Assay”:		Beziehung von Lipoprotein (a) (<i>Lp(a)</i>) zu Risikofaktoren der koronaren Herzkrankheit:
Enzymimmunasssay zur Bestimmung des Komplexes von menschlicher Granulozyten-Elastase mit α_1 -Proteinase-inhibitor	Rijn, H. J. M. van, Kruit, W. H. J. and Schrijver, J.	Erste Ergebnisse der prospektiven epidemiologischen Studie bei Betriebsangehörigen in Westfalen
693	Haptoglobin typing, is it clinically necessary for a reliable determination of haptoglobin with the single radial immunodiffusion technique?	591
Panteghini, M. and Bonora, R.	Ist die Haptoglobin-Typisierung klinisch erforderlich für eine zuverlässige Bestimmung von Haptoglobin mit der einfachen radialen Immunodiffusion?	
Evaluation of a new continuous colorimetric method for determination of serum pseudocholinesterase catalytic activity and its application to a centrifugal fast analyser	109	
Bewertung einer neuen kontinuierlichen kolorimetrischen Methode zur Bestimmung der katalytischen Aktivität von Pseudocholinesterase im Serum und ihre Anwendung an einem Zentrifugalfestivalsengerät		
671		
Panteghini, M., Malchiodi, A., Calarco, M. and Bonora, R.	Rydén, S., Hultberg, B., Isaksson, A. and Hafström, Lo	Schriewer, H., Kohnert, U. and Assmann, G.
Clinical and diagnostic significance of aspartate aminotransferase isoenzymes in sera of patients with liver diseases	Influence on plasma β -N-acetyl-D-glucosaminidase of reticuloendothelial stimulation and depression: An experimental study in rats	Determination of LDL cholesterol and LDL apolipoprotein B following precipitation of VLDL in blood serum with phosphotungstic acid/MgCl ₂
Klinische und diagnostische Bedeutung von Aspartataminotransferase-Isoenzyme im Serum von Patienten mit Lebererkrankungen	Einfluß von Stimulation und Depression des reticuloendothelialen Systems auf die katalytische Konzentration der β -N-Acetyl-D-glucosaminidase im Plasma: Eine experimentelle Untersuchung an Ratten	Bestimmung von LDL-Cholesterin und LDL-Apolipoprotein B nach Fällung von VLDL im Blutserum mittels Phosphorwolframsäure/MgCl ₂
153	219	35
Parviaainen, Markku T., Koivula, Timo and Jokela, Hannu	Sabinski, Frauke and Wosiewitz, U.	Schriewer, H., Schulte, H. and Assmann, G.
Serum amylase and isoamylase assay on the Hitachi 705 automatic clinical chemical analyzer	The sugar spectrum of human cholesterol gallstones, mixed and pigment gallstones:	HDL phosphatidyl choline and risk-factors of coronary heart disease
Bestimmung von Amylase und Isoamylase im Serum mit dem Hitachi 705	Combined quantitative analysis of neutral sugars, N-acetylhexosamines, hexuronic and N-acetylneuraminic acids by capillary gas-liquid chromatography	HDL-Phosphatidylcholin und Risikofaktoren der koronaren Herzkrankheit
41	Das Zuckerspektrum von Cholesterin-Gallensteinen, gemischten Gallensteinen und erdigen Pigment-Gallensteinen: Kombinierte quantitative Analyse der Neutralzucker, N-Acetylhexosamine, Hexuronsäuren und der N-Acetylneuraminsäure mit Hilfe der Kapillargaschromatographie	515
Passing, H. and Bablok, W.		Seeger, W., Róka, L. and Moser, U.
Comparison of several regression procedures for method comparison studies and determination of sample sizes		Detection of organic hydroperoxidases in rabbit lung lavage fluid, but not in lung tissue homogenate, using GSH peroxidase and GSH reductase
Application of linear regression procedures for method comparison studies in Clinical Chemistry, Part II		Messung organischer Hydroperoxide in Kaninchenglungen-Lavageflüssigkeit, aber nicht im Lungengewebe-Homogenat, mittels GSH-Peroxidase und GSH-Reduktase
		711

Shamberger, R. J.	
Serum sialic acid in normals and in cancer patients	
Sialinsäure im Serum von Gesunden und Patienten mit Carcinomen	647
Shin, Y. S., Stern, C., Rücker, A. v. and Endres, W.	
Glycated haemoglobin and glycated albumin:	
Evaluation of different methods in diabetic control	
Glykosyliertes Hämoglobin und glykosierte Albumin:	
Erprobung verschiedener Methoden bei der Diabeteskontrolle	47
Siekmann, L.	
Determination of oestradiol-17 β in human serum by isotope dilution-mass spectrometry	
Definitive methods in Clinical Chemistry, II	
Bestimmung von Ostradiol-17 β im menschlichen Serum mit Hilfe der massenspektrometrischen Isotopenverdünnungsanalyse	
Definitive Methods in der klinischen Chemie, II	551
Spincemaille, J., Delanghe, J., Buyzere, M. De, Breemeersch, M. and Blaton, V.	
Evaluation of three current methods for the determination of creatine kinase-MB catalytic activity	
Vergleich von drei gebräuchlichen Methoden zur Bestimmung der katalytischen Aktivität von Kreatinkinase	603
Stamm, D., Hansert, E. and Feuerlein, W.	
Detection and exclusion of alcoholism in men on the basis of clinical laboratory findings	
Erkennung oder Ausschluß des Alkoholismus bei Männern aufgrund klinisch-chemischer Befunde	79
Stamm, D., Hansert, E. and Feuerlein, W.	
Excessive consumption of alcohol in men as a biological influence factor in clinical laboratory investigations	
Der übermäßige Alkoholkonsum von Männern als Einflußgröße bei klinisch-chemischen Untersuchungen	65
Sulman, Ch., Gosselin, P., Carpentier, Ph. and Lemaire, B.	
Value of the estimation of thyroglobulin levels in the surveillance of treated differentiated thyroid carcinoma	
Der Wert der Bestimmung der Thyroglobulin-Konzentration für die Überwachung des behandelten differenzier-ten Schilddrüsencarcinoms	215
Tandt, W. R. Den and Brossmer, R.	
Determination of methylumbelliferyl-N-acetylneurameric acid sialidase for clinical purposes	
Bestimmung der Methylumbelliferyl-N-acetylneuraminsäure spaltenden sauren Sialidase für klinische Zwecke	189
Tsuboi, Seiji, Uda, Naoto, Ikeda, Mikiko, Hirota, Kazuhiro and Ohmori, Shinji	
S-(1,2-Dicarboxyethyl)glutathione and S-(1,2-dicarboxyethyl)L-cysteine in lens	
S-(1,2-Dicarboxyethyl)glutathion und S-(1,2-Dicarboxyethyl)L-cystein in der Linse des Auges	285
Uhlhaas, S. und Olek, K.	
Quantitative fluorimetriche Bestim- mung der 4-Aminobuttersäure aus Li- quor mit einem Aminosäurenanalysator	
Quantitative fluorimetric measurement of 4-aminobutyric acid in human cere- brospinal fluid with an amino acid ana- lyser	379
Weisweiler, P. and Schwandt, P.	
Determination of human apolipoproteins A-I, B, and E by laser nephelometry	
Bestimmung der Humanapoliproteine A-I, B and E durch Lasernephelo- metrie	113
Wood, W. G., Fricke, H., Haritz, J., Gadow, A., Krausz, Heidi-Susanne, Tode, Bettina, Strasburger, C. J. and Scriba, P. C.	
An evaluation of four different lumin- escence immunoassay systems:	
CELIA (chemiluminescent immuno- assay),	
SPALT (solid-phase antigen lumin- escence technique),	
ILMA (immunoluminometric assay) and ILSA (immunoluminometric labelled second antibody)	
A critical study of macro solid phase for use in immunoassay systems, Part III Beurteilung von vier verschiedenen Lu- mineszenz-Immunoassays:	
CELIA (chemiluminescent immuno- assay),	
SPALT (solid-phase antigen lumi- nescence technique),	
ILMA (immunoluminometric assay) and ILSA (immunoluminometric labelled second antibody)	
Eine kritische Untersuchung von Makro- Festphasen zum Gebrauch in Immuno- assay-Systemen, Teil III	349
Zweens, J. and Frankena, Henny	
Simultaneous determination of dimethadione and trimethadione by infrared- spectrometry:	
Application for mean intracellular pH measurement	
Simultane Bestimmung von Di- und Trimethadion durch Infrarot-Spektrometrie:	
Anwendung zur Bestimmung des mittleren intrazellulären pH	641

Short communications/Kurzmitteilungen

Harder, A., Widjaja, F. and Debuch, H.	
Studies on lipids from liver and spleen of a child (O.L.) with Niemann-Pick's disease type C	
Untersuchung der Leber- und Milzlipide eines Kindes (O.L.) mit Niemann-Pick'scher Erkrankung	199
Klingmüller, V., Bergmann, Eva und Claaßen, P.	
Alaninaminopeptidase-Ausscheidung bei Kindern: Referenzbereiche und der Einfluß nierengängiger Kontrastmittel	
The urinary excretion of alanine amino-peptidase in children: Reference values and influence of nephrotropic contrast media	787
Laing, I. A., Young, R. J. and Westwood, A.	
Biochemical observations on a non-elite marathon runner	
Biochemische Beobachtungen an einem Nicht-Elite-Marathonläufer	535
Tuttlebee, J. W.	
A comparison of automated and manual radioimmunoassays for the estimation of serum digoxin	
Vergleich von mechanisierten und ma- nuellen Radioimmunoassays für die Bestimmung von Digoxin im Serum	119
Uldall, A.	
Analyte and matrix problems in the cali- bration and quality assessment of the bromocresol green method for albumin in serum	
Analyt- und Matrix-Probleme bei der Kalibrierung und Qualitätskontrolle der Bromkresolgrün-Methode für Albumin im Serum	305
Weber, J. A.	
The enzymatic determination of urea using the Greiner G 300	
Enzymatische Bestimmung von Harn- stoff mit dem Greiner G 300	195

Workshop conference report/Kleinkonferenz-Berichte

Haeckel, R.	Statistische Probleme beim Vergleich klinisch-chemischer Analysenverfahren Bericht über die Kleinkonferenz der Deutschen Gesellschaft für Klinische Chemie am 9. und 10. Juni 1983 in Bremen	Statistical problems in the comparison of methods of clinical chemical analysis Report on the workshop conference of the German Society for Clinical Chemistry held on June 9 and 10, 1983 in Bremen
		265

IFCC Sections/IFCC-Sektionen

Bechtler, G., Haeckel, R., Lappe, H. and Tausch, W. †	Guidelines (1984) for listing specifications of spectrometers in Clinical Chemistry	Teil 3. Auswahl und Beurteilung unter Verwendung von Referenzmaterialien. Allgemeine Überlegungen	573	Beurteilung der Leistungsfähigkeit von Reagenzbestecks für die Diagnostik in Laboratorien mit begrenzten Mitteln Appendix A: Glucose	827
Richtlinien (1984) zur Auflistung von Spezifikationen von Spektrometern in der Klinischen Chemie		IFCC/WHO principles and recommendations on evaluation of diagnostic reagent sets used in health laboratories with limited resources.		PetitClerc, C. and Wilding, P.	
Logan, J. E., Bayse, D. D., Koedam, J. C., Mather, A. and Wilding, P.	IFCC/WHO principles and recommendations on evaluation of diagnostic reagent sets used in health laboratories with limited resources	Part 4. Evaluation of performance using reference materials of analytes commonly determined in blood serum or plasma	817	The theory of reference values, Part 2. Selection of individuals for the production of reference values	
Logan, J. E., Bayse, D. D., Koedam, J. C., Mather, A. and Wilding, P.	IFCC/WHO-Prinzipien und -Empfehlungen zur Beurteilung von Reagenzbestecks für die Diagnostik in Laboratorien mit begrenzten Mitteln.	Teil 4. Beurteilung der Leistungsfähigkeit mit Referenzmaterialien für gewöhnlich in Serum oder Plasma bestimmte Bestandteile		Theorie der Referenzwerte, Teil 2. Auswahl von Probanden für die Bestimmung von Referenzwerten	203
Logan, J. E., Bayse, D. D., Koedam, J. C., Mather, A. and Wilding, P.	IFCC/WHO-Prinzipien und -Empfehlungen zur Beurteilung von Reagenzbestecks für die Diagnostik in Laboratorien mit begrenzten Mitteln	Evaluation of performance of diagnostic reagent sets used in health laboratories with limited resources Appendix A: Glucose	505	Siest, G. and Dawkins, S. J.	
Logan, J. E., Bayse, D. D., Koedam, J. C., Mather, A. and Wilding, P.	Part 3. Selection and evaluation using reference materials. General considerations	A basic education and training framework for Medical Laboratory Technicians in Clinical Chemistry		Drug effects in Clinical Chemistry. Part I. The basic concepts	
Logan, J. E., Bayse, D. D., Koedam, J. C., Mather, A. and Wilding, P.	IFCC/WHO-Prinzipien und -Empfehlungen zur Beurteilung von Reagenzbestecks für die Diagnostik in Laboratorien mit begrenzten Mitteln	Rahmen für die Grundausbildung und Weiterbildung von Medizinischen Laboratoriumsassistenten in Klinischer Chemie	497	Effekte von Medikamenten in der Klinischen Chemie. Teil 1. Grundlegende Überlegungen	271
Worth, H. G. J.					

Letters to the Editors/ Briefe an die Herausgeber

On acid phosphatase in serum		
Letter	Dalen, A. van	
Reply	Seiler, D. and Tritschler, W.	
Final comment	Dalen, A. van	331
On serum total hydroxyproline assay		
Letter	Struck, H.	
Reply	Gilbertson, T. J.	
Final comment	Struck, H.	124

History of Clinical Chemistry/ Geschichte der Klinischen Chemie

Kattermann, R.	
Walter Siegfried Loewe (1884–1963)	
Sein Beitrag zur Analytik, Biologie und Pharmakologie der Sexualhormone	
Walter Siegfried Loewe (1884–1963)	
His contribution to the analysis, biology and pharmacology of the sex hormones	
	505

Honours/Ehrungen

Ladislaus Róka	
65 Jahre alt	
Ladislaus Róka	
65 years of age	703
Hansjürgen Staudinger	
70 Jahre alt	
Hansjürgen Staudinger	
70 years of age	701

Award/Preisverleihung

Preis „Biochemische Analytik“	
verliehen an E. M. Southern	
Prize “Biochemical Analysis”	
awarded to E. M. Southern	394

Workshop conference of the German Society for Clinical Chemistry Immunological Diagnostics

Bohner, J. and Stein, W. Immunological procedures in clinical enzyme diagnostics Immunologische Verfahren in der klinischen Enzymdiagnostik	Müller-Hermelink, H. K. and Hansmann, M.-L. Immunohistochemical procedures: Applications and problems Immunhistochemische Methoden: Ihre Anwendung und Probleme	943 953	Wagener, C. Diagnostic sensitivity, diagnostic specificity and predictive value of the determination of tumour markers Diagnostische Empfindlichkeit, diagnostische Spezifität und prädiktiver Wert der Bestimmung von Tumormarkern
Dwenger, A. Radioimmunoassay: An overview Radioimmunoassay: Ein Überblick	Oellerich, M. Enzyme-immunoassay: A review Enzym-Immunoassay: Eine Übersicht	883 895	969
Falkenberg, F. W., Pierard, Dany, Mai, U. and Kantwerk, Gudrun Polyclonal and monoclonal antibodies as reagents in biochemical and in clinical-chemical analysis Polyklonale und monoklonale Antikörper als Reagenzien in der biochemischen und klinisch-chemischen Analytik	Valet, G., Rüssmann, L. and Wirsching, R. Automated flow-cytometric identification of colo-rectal tumour cells by simultaneous DNA, CEA-antibody and cell volume measurements Automatische Identifizierung kolorektaler Tumorzellen mit Hilfe simultaner durchflußzytometrischer Messung von DNA, CEA-Antikörpern und Zellvolumen	867 935	Wönigkeit, K. Diagnostic concepts in clinical organ transplantation: Histocompatibility testing and T cell monitoring Immunologische Diagnostik bei Organtransplantationen: Histokompatibilitätstestung und T-Zell-Monitoring
Henkel, E. Marker-free immunological analytical methods Markerfreie immunologische Analysenverfahren	Vogt, W. An evaluation of immunological methods based on the requirements of the Clinical Chemist Wertigkeit immunologischer Methoden aus der Sicht des Klinischen Chemikers	919 927	Wood, W. G. Luminescence immunoassays: Problems and possibilities Lumineszenz-Immunoassays: Probleme und Anwendung
Kuss, E. Physikalisch-chemische Aspekte immunologischer und anderer reversibler Assoziations-Reaktionen Physical chemical aspects of immunological reactions and other reversible associations		851	905

Recommendations of the German Society for Clinical Chemistry/ Empfehlungen der Deutschen Gesellschaft für Klinische Chemie

Durchführung klinisch-chemischer Untersuchungen bei der Prüfung von Arzneimitteln Performance of clinical-chemical tests on pharmaceuticals	811
--	-----

Obituary/Nachruf

In memoriam Ivar Trautschold	847
------------------------------	-----

Acknowledgement / Danksagung

Acknowledgement/Danksagung	980
----------------------------	-----

Recommendations of the Deutsche Forschungsgemeinschaft/ Empfehlungen der Deutschen Forschungsgemeinschaft

Empfehlungen für die Installation einer Gaschromatographie-Massenspektrometrie-Kopplung für klinisch-toxikologische Laboratorien Recommendations for the installation of a gas chromatography/mass spectrometry combination for clinical toxicological laboratories	699
--	-----

Guest Editorial/Gast-Editorial

Oellerich, M. Workshop conference of the German Society for Clinical Chemistry Immunological Diagnostics Introduction Kleinkonferenz der Deutschen Gesellschaft für Klinische Chemie Immunologische Diagnostik Einführung	845
---	-----

Erratum

Im Beitrag von E. Kuss, diese Z. 22, 1984, pp. 851–865 muß der Name Kirchoff richtig lauten Kirchhoff. In the paper by E. Kuss, this j. 22, 1984 pp. 851–865 the name Kirchoff should read Kirchhoff.
--

Book Reviews/Buchbesprechungen

Allen, R. C., Bienvenu, J., Laurent, P. and Suskind, R. M. Marker Proteins in Inflammation	Brown, S. N. An Introduction to Spectroscopy for Biochemists	502 447	Drazil, J. v. Quantities and Units of Measurement. A Dictionary and Handbook
Beal, J. L. and Reinhard, E. Natural Products as Medicinal Agents	Brown, S. S. and Davies, D. S. Organ-Directed Toxicity – Chemical Indices and Mechanisms – Proceedings of the Symposium on Chemical Indices and Mechanisms of Organ-Directed Toxicity, Barcelona, 4–7 March 1981	448 503	Eastham, R. D. D. Interpretation klinisch-chemischer Laborresultate. 2. Aufl.
Bertsch, W., Jennings, W. G. and Kaiser, R. E. Recent Advances in Capillary Gas Chromatography. Vols. 1 and 2.	Engel, P. C. Enzyme Kinetics – The Steady-State Approach. 2nd Edition	583 447	

Gräsbeck, R. and Alström, T. Reference Values in Laboratory Medicine. The Current State of the Art. 583	Klämbt, D. and Heitmann, I. Grundriß der Molekularbiologie 503	Rosenfeld, L. Origins of Clinical Chemistry. The Evolution of Protein Analysis 447
Gut, I., Cikri, M. and Plaa, G. L. Proceedings in Life Sciences. Industrial and Environmental Xenobiotics Metabolism and Pharmacokinetics of Organic Chemistry and Metals 502	Lamy, J. and Lamy, J. Invertebrate Oxygen-Binding Proteins. Structure, Active Site, and Function 502	Stich, H. F. and San, R. H. C. Topics in Environmental Physiology and Medicine. Short-Term Tests for Chemical Carcinogens 448
Karow, A. M. and Pegg, D. E. Organ Preservation for Transplantation. 2nd Edition 503	Miescher, P. A., Bolis, L. and Torrigiani, G. The Menarini Series on Immunopathology. Vol. 3. Immunogenetics 583	

General Index/Gesamtregister

Authors' Index/Autorenregister

- Agabiti-Rosei, E. 539
 Allner, R. 759
 Amadio, P. 147
 Assink, H. A. 685
 Assmann, G. 397, 585, 781
 Assmann, G. s. Kattermann, R. 245
 Assmann, G. s. Schriewer, H. 35, 515, 591
 Bablok, W. s. Passing, H. 431
 Bäßler, K. H. s. Neuhäuser, M. 731
 Balcke, P. 261
 Bauersfeld, W. s. Knoll, E. 597
 Bayse, D. D. s. Logan, J. E. 573, 817, 827
 Bechtler, G. 565
 Becker, J. U. 389
 Beneking, M. s. Külpmann, W. R. 773
 Bergmann, E. s. Klingmüller, V. 787
 Beschi, M. s. Agabiti-Rosei, E. 539
 Biber, A. 185
 Björkhem, I. s. Kattermann, R. 245
 Blaton, V. s. Spincemaille, J. 603
 Bleyl, H. s. Golf, S. W. 723
 Bliersbach, Y. s. Schädlich, H.-J. 483
 Blijenberg, B. G. 609
 Blijenberg, B. G. s. Assink, H. A. 685
 Bödeker, R. s. Golf, S. W. 723
 Boerma, G. s. Assink, H. A. 685
 Boerma, G. s. Kattermann, R. 245
 Börnsen, S. s. Dörner, K. 419
 Bohner, J. 943
 Bollengier, F. 653
 Bonora, R. s. Panteghini, M. 153, 671
 Boos, K.-S. s. Hagemeier, E. 175
 Borner, K. s. Kattermann, R. 245
 Bosch, A. M. G. 29
 Bossmann, B. 449
 Brätter, P. s. Gardiner, P. E. 159
 Brechbühler, T. 301
 Breemeersch, M. s. Spincemaille, J. 603
 Breuer, N. 623
 Brombacher, P. J. s. Costongs, G. M. P. J. 613
 Brossmer, R. s. Tandt, W. R. Den 189
 Brouwer, H. J. s. Blijenberg, B. C. 609
 Bruchelt, G. 1
 Brüstle, A. s. Golf, S. W. 723
 Büttner, D. s. Lindena, J. 97
 Büttner, G. s. Assmann, G. 585
 Bützow, G. H. s. Rehpenning, W. 319
 Butterly, J. E. s. Ratnaike, R. N. 105
 Buyzere, M. De s. Spincemaille, J. 603
 Calarco, M. s. Panteghini, M. 153
 Campos, R. s. Dörner, K. 419
 Carpentier, Ph. s. Sulman, Ch. 215
 Castellano, M. s. Agabiti-Rosei, E. 539
 Claassen, P. s. Klingmüller, V. 787
 Clinet, G. s. Bollengier, F. 653
 Costongs, G. M. P. J. 613
 Dalen, A. van 331, 333
 Dawkins, S. J. s. Siest, G. 271
 Debuch, H. s. Harder, A. 199
 Delanghe, J. s. Spincemaille, J. 603
 Delbrück, A. s. Dresow, B. 527
 Delmotte, P. s. Bollengier, F. 653
 Desager, J. P. s. Kattermann, R. 245
 Ditschuneit, H. s. Hutt, V. 141
 Dittel, K. D. s. Mössner, E. 467
 Dörner, K. 419
 Dommes, P. s. Breuer, N. 623
 Dresow, B. 527
 Dwenger, A. 883
 Endler, A. T. s. Lapin, A. 53
 Endres, W. s. Shin, Y. S. 47
 Falk, U. 661
 Falkenberg, F. W. 867
 Fateh-Moghadam, A. s. Knüppel, W. 407
 Federkiel, H. s. Hansert, E. 791
 Felgenhauer, K. s. Schädlich, H.-J. 483
 Feuerlein, W. s. Stamm, D. 65, 79
 Fogh-Andersen, N. 479
 Franken, H. s. Zweens, J. 641
 Fricke, H. s. Gadow, A. 337
 Fricke, H. s. Wood, W. G. 349
 Fujita, T. s. Matsumoto, A. 281
 Gabl, F. s. Lapin, A. 53
 Gadow, A. 337
 Gadow, A. s. Wood, W. G. 349
 Galteau, M. M. 275
 Gardiner, P. E. 159
 Garth, H. 769
 Gatta, A. s. Amadio, P. 147
 Gessner, H. s. Gardiner, P. E. 159
 Gey, S. s. Külpmann, W. R. 773
 Gilbertson, T. J. 124
 Goebell, H. s. Breuer, N. 623
 Göttmann, U. s. Neuhäuser, M. 731
 Golf, S. W. 705, 717, 723, 751
 Gosselin, P. s. Sulman, Ch. 215
 Graben, N. s. Kreuzfelder, E. 61
 Graef, V. s. Golf, S. W. 705, 717
 Gressner, A. M. 237, 633
 Grill, H.-J. s. Manz, B. 209
 Gruber, W. s. Nägele, U. 165
 Gruhl, H. 385
 Guder, W. G. 129
 Günther, T. 473
 Gunzer, G. s. Neumann, S. 693
 Hadžija, M. s. Juretić, D. 21
 Haeckel, R. s. Bechtler, G. 565
 Hafström, L. s. Rydén, S. 219
 Hägele, E. O. s. Nägele, U. 165
 Hagemeier, E. 175
 Hansert, E. 791
 Hansert, E. s. Stamm, D. 65, 79
 Hansmann, M.-L. s. Müller-Hermelink, H. K. 953
 Happel, O. s. Golf, S. W. 717
 Hara, K. s. Hijikata, Y. 291
 Harder, A. 199
 Haritz, J. s. Wood, W. G. 349
 Harm, K. s. Rehpenning, W. 319
 Harwengt, C. s. Kattermann, R. 245
 Haschen, R. J. s. Bossmann, B. 449
 Haubenstock, A. s. Balcke, P. 261
 Heber, F. s. Kreuzfelder, E. 61
 Heinemann, G. 229
 Heinrich, D. s. Golf, S. W. 723
 Hempel, K. s. Biber, A. 185
 Henkel, E. 489, 919
 Henkel, R. s. Henkel, E. 489
 Hennrich, N. s. Neumann, S. 693
 Heubner, A. s. Manz, B. 209
 Hijikata, Y. 291
 Hirota, K. s. Tsuboi, S. 285
 Hockeborn, M. s. Rick, W. 357
 Höfeler, H. 15
 Hoffmann, S. s. Ratnaike, R. N. 105
 Hohenwallner, W. s. Scholer, A. 677
 Hüfner, M. s. Falk, U. 661
 Hultberg, B. s. Masson, P. 427
 Hultberg, B. s. Rydén, S. 219
 Hutt, V. 141
 Ikeda, M. s. Tsuboi, S. 285
 Isaksson, A. s. Rydén, S. 219
 Jabs, H.-U. s. Assmann, G. 781
 Janson, P. C. W. s. Costongs, G. M. P. J. 613
 Javeri, S. 735
 Jaworek, D. s. Kattermann, R. 245
 Jelić, Z. 559
 Johnson, B. F. s. Marwaha, R. K. 403
 Jokela, H. s. Parviaainen, M. T. 41
 Jung, K. 523
 Juretić, D. 21
 Kaeslin, M. s. Brechbühler, T. 301
 Kantwerk, G. s. Falkenberg, F. W. 867
 Kattermann, R. 245, 505
 Kaul-Kunz, C. s. Golf, S. W. 751
 Kemper, K. s. Hagemeier, E. 175
 Kempf, K. D. s. Golf, S. W. 723
 Kladetzky, R. G. s. Assmann, G. 585
 Klemens, M. s. Kochen, W. 309
 Kley, H. K. 371, 461
 Klingemann, H.-G. s. Höfeler, H. 15
 Klingmüller, V. 787
 Klör, H. U. s. Hutt, V. 141
 Knedel, M. s. Knüppel, W. 407
 Knoll, E. 597, 741
 Knüppel, W. 407
 Kochen, W. 309
 Koedam, J. C. s. Logan, J. E. 573, 817, 827
 Kohl, B. s. Külpmann, W. R. 773
 Kohnert, U. s. Schriewer, H. 35
 Koivula, T. s. Parviaainen, M. T. 41
 Kopsa, H. s. Balcke, P. 261
 Kossmann, K. T. 253
 Krausz, H.-S. s. Wood, W. G. 349
 Kreienberg, R. s. Manz, B. 209
 Kreuzfelder, E. 61
 Krüsken, H. L. s. Kley, H. K. 461
 Kruit, W. H. J. s. Rijn, H. J. M. van 109
 Külpmann, W. R. 773
 Kupke, I. s. Kattermann, R. 245
 Kuss, E. 851
 Kuwert, E. s. Kreuzfelder, E. 61
 Ladefoged, J. s. Fogh-Andersen, N. 479
 Laing, I. A. 535
 Lang, H. s. Neumann, S. 693
 Lapin, A. 53
 Lappe, H. s. Bechtler, G. 565
 Lehmann, P. s. Nägele, U. 165

- Leijnse, B. s. Assink, H. A. 685
 Leijnse, B. s. Blijenberg, B. G. 609
 Leijnse, B. s. Kattermann, R. 245
 Lemaire, B. s. Sulman, Ch. 215
 Lindena, J. 97
 Lipovac, K. s. Juretić, D. 21
 Lizana, J. 545
 Logan, J. E. 573, 817, 827

 Maass, G. s. Vogel, R. 847
 Mahler, A. s. Bollengier, F. 653
 Mai, U. s. Falkenberg, F. W. 867
 Majkić-Singh, N. s. Jelić, Z. 559
 Malchiodi, A. s. Panteghini, M. 153
 Manz, B. 209
 Marwaha, R. K. 403
 Masson, P. 427
 Mather, A. s. Logan, J. E. 573, 817, 827
 Matsumoto, A. 281
 Mayer, H. s. Gruhl, H. 385
 Menzl, H. J. s. Assmann, G. 585
 Merker, H. J. s. Günther, T. 473
 Möller, G. s. Kattermann, R. 245
 Møller-Petersen, J. s. Fogh-Andersen, N. 479
 Mössner, E. 467
 Morich, S. s. Henkel, E. 489
 Moser, U. s. Seeger, W. 711
 Müller, F. W. s. Knoll, E. 597
 Müller-Hermelink, H. K. 953
 Murata, K. s. Hijikata, Y. 291

 Nägele, U. 165
 Neuhäuser, M. 731
 Neumann, S. 693
 Neumeier, D. s. Knüppel, W. 407
 Nolte, W. s. Assmann, G. 781
 Nürnberg, H. W. s. Gardiner, P. E. 159

 Oellerich, M. 845, 895
 Oellerich, M. s. Külpmann, W. R. 773
 Ogunyemi, E. O. s. Lapin, A. 53
 Ohmori, S. s. Tsuboi, S. 285
 Olek, K. s. Uhlhaas, S. 379
 Olsson, I. s. Lizana, J. 545

 Panteghini, M. 153, 671
 Parviainen, M. T. 41
 Passing, H. 431
 Peltzer, B. s. Gressner, A. M. 633
 Pergande, M. s. Jung, K. 523
 PetitClerc, C. 203
 Pfleiderer, G. s. Mössner, E. 467
 Pierard, D. s. Falkenberg, F. W. 867
 Pistor, K. s. Kreuzfelder, E. 61
 Pollow, K. s. Manz, B. 209
 Pürschel, S. s. Guder, W. G. 129

 Ratge, D. s. Knoll, E. 597
 Ratnaike, R. N. 105
 Rehder, M. s. Manz, B. 209
 Rehpenning, W. 319
 Reinholdt, C. s. Jung, K. 523
 Richter, F. s. Heinemann, G. 229
 Rick, W. 357
 Rick, W. s. Kley, H. K. 371
 Rijn, H. J. M. van 109
 Ringe, J.-D. s. Rehpenning, W. 319
 Roetering, H. A. s. Blijenberg, B. G. 609
 Róka, L. s. Golf, S. W. 751
 Róka, L. s. Seeger, W. 711
 Rücker, A. v. s. Shin, Y. S. 47
 Rüssmann, L. s. Valet, G. 935
 Ruol, A. s. Asmodio, P. 147
 Rydén, S. 219

 Sabinski, F. 453
 Sameshima, Y. s. Hijikata, Y. 291
 Sandkamp, M. s. Schriewer, H. 591
 Sauer, G. s. Nägele, U. 165
 Schädlich, H.-J. 483
 Schievelbein, H. s. Heinemann, G. 229
 Schifferdecker, M. s. Schädlich, H.-J. 483
 Schlaghecke, R. s. Kley, H. K. 461
 Schleicher, E. 223
 Schlimme, E. s. Hagemeier, E. 175
 Schmidt, K. H. s. Bruchelt, G. 1
 Schmidt, P. s. Balcke, P. 261
 Schmidt-Gayk, H. s. Falk, U. 661

 Scholer, A. 677
 Scholz, D. s. Jung, K. 523
 Schriewer, H. 35, 515, 591
 Schriewer, H. s. Assmann, G. 397, 781
 Schrijver, J. s. Rijn, H. J. M. van 109
 Schulte, H. s. Assmann, G. 397
 Schulte, H. s. Schriewer, H. 515, 591
 Schulze, B. s. Jung, K. 523
 Schwandt, P. s. Weisweiler, P. 113
 Scriba, P. C. s. Wood, W. G. 349
 Seeger, W. 711
 Seiler, D. 331
 Seim, K. E. s. Golf, S. W. 717
 Shamberger, R. J. 647
 Shin, Y. S. 47
 Shiozaki, Y. s. Hijikata, Y. 291
 Siekmann, L. 551
 Siest, G. 271
 Siest, G. s. Galteau, M. M. 275
 Signorini, C. s. Agabiti-Rosei, E. 539
 Slijepčević, M. s. Juretić, D. 21
 Spasić, S. s. Jelić, Z. 559
 Spincemaille, J. 603
 Sprunck, H. P. s. Kochen, W. 309
 Stamm, D. 65, 79
 Stamm, D. s. Hansert, E. 791
 Stein, W. s. Bohner, J. 943
 Stern, C. s. Shin, Y. S. 47
 Stoeppler, M. s. Gardiner, P. E. 159
 Strasburger, C. J. s. Gadow, A. 337
 Strasburger, C. J. s. Wood, W. G. 349
 Strobelt, V. s. Jung, K. 523
 Struck, H. 123, 125
 Sulman, Ch. 215
 Svensson, L. s. Kattermann, R. 245

 Tandon, R. s. Breuer, N. 623
 Tandt, W. R. Den 189
 Tausch, W. † s. Bechtler, G. 565
 Tauscher, B. s. Kochen, W. 309
 Temme, H. s. Golf, S. W. 723
 Tode, B. s. Wood, W. G. 349
 Todorović, P. s. Jelić, Z. 559
 Tosoni, S. s. Agabiti-Rosei, E. 539
 Trautschold, I. s. Lindena, J. 97
 Trinder, P. s. Kattermann, R. 245

 Tritschler, W. s. Seiler, D. 331
 Tsuboi, S. 285
 Tuttlebee, J. W. 119

 Uda, N. s. Tsubori, S. 285
 Uhlhaas, S. 379
 Uhlenbrück, G. s. Javeri, S. 735
 Uldall, A. 305

 Valet, G. 935
 Vandewalle, A. s. Guder, W. G. 129
 Vogel, R. 847
 Vogt, W. 927
 Voigt, K. D. s. Rehpenning, W. 319
 Vormann, J. s. Günther, T. 473

 Wagener, C. 969
 Wahlefeld, A. W. s. Nägele, U. 165
 Weber, J. A. 195
 Wechsler, J. G. s. Hutt, V. 141
 Weisweiler, P. 113
 Westwood, A. s. Laing, I. A. 535
 Widjaja, F. s. Harder, A. 199
 Wiedemann, E. s. Nägele, U. 165
 Wieland, O. H. s. Schleicher, E. 223
 Wilding, P. s. Logan, J. E. 573, 817, 827
 Wilding, P. s. PetitClerc, C. 203
 Windeck, R. s. Kreuzfelder, E. 61
 Wirsching, R. s. Valet, G. 935
 Wirthensohn, G. s. Guder, W. G. 129
 Wisser, H. s. Knoll, E. 597, 741
 Wonigkeit, K. 959
 Wood, W. G. 349, 905
 Wood, W. G. s. Gadow, A. 337
 Worth, H. G. J. 497
 Wosiewitz, U. s. Sabinski, F. 453
 Wyler, F. s. Brechbühler, T. 301

 Zazgornik, J. s. Balcke, P. 261
 Živanov-Stakić, D. s. Jelić, Z. 559
 Zoch, E. s. Garth, H. 769
 Zweens, J. 641

 Young, R. J. s. Laing, I. A. 535

Subject Index/Sachregister

- ABEI-H 337, 349
 absorbance
 –, molar lineic 489
 –, 2-chloro-4-nitrophenol 489
 accuracy
 –, radioimmunoassay 883

 β-N-acetyl-D-glucosaminidase
 –, kidney 21
 –, diabetes mellitus 21
 –, plasma 219
 –, urine 21
 –, diabetes mellitus 21
 acetylsalicylic acid 559

 acetylsalicylic acid
 –, interference 559
 –, enzyme assays 559
 acidic α₁-glycoprotein
 –, myocardial infarction 723
 –, fibrinolysis by streptokinase 723

 acridine 905
 action pattern
 –, α-amylase 427
 activation energy
 –, triglyceride hydrolysis 357
 –, by lipase 357
 Adair equation 851

- adenosine
 -, assay 175
 adenosine deaminase
 -, pH-stat method 769
 adenyl cyclase
 -, regulatory component 281
 --, erythrocyte 281
 adrenaline 539
 affinity
 -, definition 851
 age dependence
 -, laboratory values 613
 alanine aminopeptidase
 -, brush border membrane 449
 -, urine 523, 787
 --, and contrast media 787
 alanine aminotransferase 153
 -, assay 559
 --, drug interference 559
 -, myocardial infarction 723
 --, fibrinolysis by streptokinase 723
 albumin
 -, bromocresol green 685
 -, bromocresol purple 685
 -, glycation 223
 -, glycated 47
 -, plasma 301
 --, minipig 301
 -, serum 305
 --, bromocresol green method 305
 albuminuria 223
 alcohol
 -, consumption, excessive 65
 --, influence factor 65
 --, biological 65
 alcoholism
 -, clinical laboratory findings 791
 -, detection 791
 --, clinical laboratory findings 791
 -, frequency 79
 -, men 79
 --, detection 79
 --, by clinical laboratory findings 79
 --, exclusion 79
 --, by clinical laboratory findings 79
 aldosterone
 -, blood 371
 -, plasma 371, 717
 --, physical exercise 717
Allen-Doisy test 505
 AMETIA 895
 amidolytic assay
 -, proteinase inhibitors 633
 amino acids
 -, metabolism 535
 --, marathon runner 535
 4-aminobutyric acid
 -, cerebrospinal fluid 379
 --, fluorimetry 379
 aminophenazone
 -, interference 559
 --, enzyme assays 559
 ammonia
 -, blood 105
 --, reflectometer 105
 amylase
 -, inhibitor 41
 --, wheat 41
- amylose
 -, serum 41
 --, *p*-nitrophenyl- α -D-maltoheptaoside 41
 α -amylase
 -, assay 677
 --, *p*-nitrophenylheptaoside 677
 -, serum 427, 489
 --, 2-chloro-4-nitrophenyl- β -D-maltoheptaoside 489
 --, *p*-nitrophenyl-maltoheptaoside 427
 ---, action pattern 427
 -, urine 489
 --, 2-chloro-4-nitrophenyl- β -D-maltoheptaoside 489
 analgesics
 -, interference 559
 --, enzyme assays 559
 analytes
 -, determination 65
 --, influence factor 65
 ---, alcohol consumption 65
 androgens
 -, detection methods 505
 androst-4-en-17 β -ol-3,11-dione
 -, plasma 461
 --, radioimmunoassay 461
 androstenedione
 -, blood 371
 -, plasma 371
 antibodies
 -, immobilized 337
 -, monoclonal 867, 943, 953, 959
 --, applications 867
 --, as reagents 867
 --, human 867
 --, preparation 867
 --, production 867
 --, purification 867
 --, rat 867
 --, polyclonal 867, 943, 953
 --, as reagents 867
 antigen
 -, epitopes 851
 -, factor VIII-related 15
 -, preparation 741
 --, catecholamines 741
 antigen antibody reaction 919
 antigens
 -, enzymes 943
 -, immobilized 337
 --, lymphocyte differentiation 867
 -, surface 959
 --, lymphocytes 959
 -, tissue 867
 --, kidney 867
 --, transplantation 959
 -, tumour 867
 -, urinary 867
 antirheumatics
 -, interference 559
 --, enzyme assays 559
 antisera
 -, catecholamines 741
 --, specificity 741
 α_1 -antitrypsin see also
 α_1 -proteinase inhibitor 653
- apolipoprotein A-I
 -, HDL 397
 --, laser nephelometry 113
 --, mutants 585
 apolipoprotein B
 -, laser nephelometry 113
 -, LDL 35
 apolipoprotein E
 -, laser nephelometry 113
Arrhenius equation 851
Arrhenius plot
 -, lipase 357
 aspartate aminotransferase
 -, assay 559
 --, drug interference 559
 -, cytosolic 723
 --, myocardial infarction 723
 ---, fibrinolysis by streptokinase 723
 --, isoenzymes 153
 --, serum 153
 --, liver disease 153
 -, mitochondrial 723
 --, myocardial infarction 723
 --, fibrinolysis by streptokinase 723
 -, total 723
 --, myocardial infarction 723
 ---, fibrinolysis by streptokinase 723
 assessment
 -, longitudinal 613
 --, laboratory values 613
 association reactions
 -, reversible 851
 --, physical-chemical aspects 851
 automation
 -, radioimmunoassay 883
 avidin
 -, biotin system 953
 avidity
 -, definition 851
Avogadro number 851
- basement membrane
 -, glomerular 223
 --, diabetes mellitus 223
 -, glycation 223
Bayes' theorem 96
 bifunctional reagents 337
 bile acids
 -, chromatography 623
 -, faeces 623
 bilirubin
 -, neonatal 609
 --, survey 609
 bioassay
 -, analytical performance 927
 bioluminescence 337, 905
 bioluminescence assay
 -, enzymes 129
 --, nephron 129
 biotin avidin system 953
 bis(monoacylglycerol)phosphate
 -, liver 199
 --, spleen 199
 bis(monoacylglycerol)phospholipid
 -, liver 199
 --, *Niemann-Pick's* disease 199
- bis(monoacylglycerol)phospholipid
 -, spleen 199
 --, *Niemann-Pick's* disease 199
 blastogenesis
 -, inhibition 209
 --, 17 β -carboxamide 209
 blood
 -, ammonia 105
 --, reflectometer 105
 -, CO 229
 --, CO-Hb 229
 -, constituents 301
 --, minipigs 301
 ---, reference values 301
 -, steroids 371
 --, influence of storage 371
 body functions
 -, investigation 811
 body weight
 -, loss 535
 --, marathon runner 535
 Boltzmann constant 851
 boronic acid affinity chromatography 175
 brain
 -, calmodulin 185
 breast carcinoma
 -, phosphatase, alkaline 467
 --, placental 467
 bromocresol green
 -, albumin 305, 685
 --, determination 305
 bromocresol purple
 -, albumin 685
 --, determination 685
 brush border membrane
 -, enzymes 449
 --, synthesis 449
- C-reactive protein
 -, ILSA 349
 caeruloplasmin
 -, SPALT 349
 caffeine
 -, interference 559
 --, enzyme assays 559
 calcium
 -, plasma 301, 717
 --, minipig 301
 --, physical exercise 717
 -, sweat 717
 --, physical exercise 717
 -, urine 717
 --, physical exercise 717
 calibration standard
 -, glucose 827
 calmodulin
 -, brain 185
 -, radioimmunoassay 185
 cancer
 -, colo-rectal 935
 --, identification 935
 -, prostate 331
 - sialic acid 647
 --, serum 647
- N6-(carbamoyl-threonyl)-adenosine 175
 carbodiimides 905
 carbohydrates
 -, gallstones 453
 -, gas chromatography 453
 carbon monoxide
 -, smokers 229

- carbon tetrachloride
 -, poisoning 633
 --, enzymes 633
 ---, serum 633
 ---, proteinase inhibitors 633
 ---, serum 633
 carbonic anhydrase 159
 17 β -carboxamide steroids
 -, blastogenesis inhibition 209
 γ -carboxyglutamic acid 123
 carboxyhaemoglobin
 -, smokers 229
 carcinoembryonic antigen 647
 carcinoma
 -, proteinase inhibitors 633
 --, serum 633
 -, thyroid 661
 ---, thyroglobulin 661
 ---, serum 661
 cataract
 -, formation 285
 --, by galactose 285
 catecholamines
 -, antigen preparation 741
 -, antisera 741
 -, radioimmunoassay 741
 -, plasma 539, 597
 --, and food intake 597
 --, assay 539
 ---, method comparison 539
 CEA 969
 CEA antibody
 -, cell 935
 --, tumour 935
 CELIA 349, 905
 Celite 29
 cell
 -, tumour 935
 -, CEA antibody 935
 -, DNA 935
 -, volume 935
 cerebrospinal fluid
 -, 4-aminobutyric acid 379
 --, fluorimetry 379
 -, lymphocytes 483
 --, IgG synthesis 483
 ---, multiple sclerosis 483
 ---, non-inflammatory diseases 483
 -, procollagen type III pro-peptide 237
 checklist
 -, laboratory needs 573
 -, product features 573
 chemiluminescence 337, 905
 -, during phagocytosis 1
 --, by granulocytes 1
 chenodeoxycholic acid 623
 children
 -, alanine aminopeptidase 787
 --, urine 787
 ---, reference range 787
 chloride
 -, plasma 301
 --, minipig 301
 2-chloro-4-nitrophenol
 -, absorbance, molar lineic 489
 -, dissociation curve 489
 2-chloro-4-nitrophenyl- β -D-malto-heptaoside
 -, substrate 489
 --, α -amylase 489
 cholesterol
 -, ester 245
 --, cleavage 245
 -, HDL 113, 397, 515
 -, LDL 35, 113, 781
 --, method comparison 781
 -, method comparison 245
 -, plasma 245, 301
 --, enzymatic determination 245
 ---, multicentre study 245
 --, minipig 301
 -, serum 245
 --, enzymatic determination 245
 ---, multicentre study 245
 -, VLDL 113
 cholic acid 623
 cholinesterase 671
 chromatography
 -, bile acids 623
 -, steroids 29
 chromogenic substrate 633
 cigarette smoking
 -, HDL apolipoprotein A-I 397
 -, HDL cholesterol 397
 clinical laboratory findings
 -, alcoholism 65, 79
 colipase 357
 collagen
 -, synthesis 527
 --, stimulation by platelet growth factor 527
 colo-rectal cancer
 -, cells 935
 --, identification 935
 constituent
 -, combination 791
 contrast media
 -, X-ray 787
 --, and alanine aminopeptidase excretion 787
 coronary heart disease
 -, risk factors 515, 591
 cortisol
 -, blood 371
 -, free 371
 --, blood 371
 --, plasma 371
 -, plasma 371 597, 717
 --, daily periodicity 597
 --, and food intake 597
 --, physical exercise 717
 -, SPALT 349
 costs
 -, analysis 927
 creatine kinase
 -, assay 559
 --, drug interference 559
 -, isoenzyme MB 603, 723, 751
 --, and serum matrix 751
 --, method comparison 603, 751
 --, myocardial infarction 603, 723
 ---, fibrinolysis by streptokinase 723
 --, myocardial infarction 723
 --, fibrinolysis by streptokinase 723
 creatinine
 -, myocardial infarction 723
 --, fibrinolysis by streptokinase 723
 creatinine
 -, plasma 301
 --, minipig 301
 creatinine
 -, plasma 301
 --, minipig 301
 creatinine
 -, urine 731
 --, and food composition 731
 critical difference 613
 curve fitting
 -, enzyme immunoassay 895
 cytidine
 -, assay 175
 cytological regeneration test 505
 daily periodicity
 -, cortisol 597
 data
 -, evaluation 319
 --, multivariate 319
 -, processing 407
 --, electrophoresis 407
 decision making 791
 definitive method
 -, oestradiol-17 β 551
 dehydroepiandrosterone sulfate
 -, blood 371
 -, plasma 371
 density, mass
 -, urine 419
 deoxycholic acid 623
 detection limits
 -, analytical methods 927
 diabetes mellitus
 -, albumin 47
 --, glycated 47
 -, basement membrane 223
 --, glomerular 223
 -, haemoglobin 47
 --, glycated 47
 -, hyperglycaemia 21
 --, and glycosidases 21
 --, kidney 21
 --, urine 21
 -, nephropathy 21
 -, proteinase inhibitors 633
 --, serum 633
 -, therapy control 47
 diagnostic efficiency 79
 diagnostic performance
 -, tumour markers 969
 diagnostic reagents sets
 -, evaluation 573
 -, performance, analytical 573
 -, practicability 573
 -, selection 573
 diagnostic sensitivity 79
 diagnostic specificity 79
 diagnostic test criteria 969
 diagnostic value
 -, haptoglobin typing 109
 diazoisoluminol 905
 dibucaine number 671
 S-(1,2-dicarboxyethyl)l-cysteine
 -, lens 285
 S-(1,2-dicarboxyethyl)glutathione
 -, lens 285
 3,4-dichlorophenylethylamine
 -, antigen preparation 741
 diclofenac
 -, interference 559
 --, enzyme assays 559
- difference
 -, critical 613
 dixogin
 -, enzyme immunoassay 759
 --, interference 759
 --, by immunoglobulins 759
 --, by rheumatoid factors 759
 -, serum 119
 --, radioimmunoassay 119
 -, urine 403
 --, radioimmunoassay 403
 dimethadione
 -, infrared spectrometry 641
 3,4-dimethoxyphenylethylamine
 -, radioimmunoassay 741
 N6-dimethyladenosine
 -, assay 175
 N2-dimethylgluanosine
 -, assay 175
 discrimination
 -, between two populations 791
 --, by multivariate decision limits 791
 dissociation curve
 -, 2-chloro-4-nitrophenol 489
 --, 4-nitrophenol 489
 distribution free methods
 -, data evaluation 319
 DNA
 -, cell 935
 --, tumour 935
 dopamine
 -, antigen preparation 741
 -, plasma 597
 -, radioimmunoassay 741
 drug
 -, effects 271, 275
 --, in clinical chemistry 271, 275
 -, monitoring 271
 drug interference 559
 duration
 -, analysis 927
- ECIA 895
 education
 -, technicians 497
 EEIA 895
 efficiency
 -, diagnostic 79, 229
 EIA 905
Ekins equation 851, 883
 elastase
 -, leukocytes 693
 --, α_1 -proteinase inhibitor complex 693
 electrolytes
 -, physical exercise 717
 electrophoresis see also gel electrophoresis 253
 -, interpretation, computer assisted 407
 -, two dimensional 53
 --, clinical application 53
 --, paraproteins 53
 --, characterization 53
 ELISA 895
 EMIT 895
 EMMIA 895

- enteropeptidase
 --, brush-border membrane 449
 enzyme
 --, assays 559
 ---, interference 559
 ---, by drugs 559
 --, catalytic assay 943
 --, diagnostics 943
 --, immunoabsorption 943
 --, immunoassay 559, 693, 759, 895, 943
 ---, application 895
 ---, competitive 895
 ---, coupling procedures 895
 ---, curve fitting 895
 ---, digoxin 759
 ---, interference 759
 ----, by immunoglobulins 759
 ----, by rheumatoid factors 759
 ---, elastase- α -proteinase 693
 ---, elastase- α_1 -proteinase inhibitor complex 693
 ---, enzyme-labels 895
 ---, future trends 895
 ---, heterogeneous 895
 ---, homogeneous 895
 ---, principles 895
 --, immunoinhibition 943
 --, immunoprecipitation 943
 --, mass determination 943
 --, radioimmunoassay 943
 enzymes
 --, bioluminescence assay 129
 --, brush border membrane 449
 --, synthesis 449
 --, label 895
 --, immunoassay 895
 --, plasma 97
 --, rat 97
 --, urine 523
 epinephrine
 --, plasma 597
 ERMA 895
 erythrocytes
 --, adenyl cyclase 281
 --, magnesium 717
 --, membrane protein 281
 --, abnormalities 281
 ---, pseudohypoparathyroidism type 1 281
 --, zinc 159
 evaluation
 --, diagnostic reagent sets 573
 --, interference 275
 --, by drugs 275
 --, kits 817, 827
 --, longitudinal 613
 --, laboratory values 613
 --, multivariate 319
 --, data 319
 --, performance 817, 827
 --, reference ranges 319
 exercise
 --, physical 717
 --, Mg supplementation 717
 ---, aldosterone 717
 ---, cortisol 717
 ---, electrolytes 717
 extraction
 --, parathyroid 479
- factor VIII-related antigen
 --, plasma 15
 ---, acute liver failure 15
 ---, liver cirrhosis 15
 faeces
 --, bile acids 623
 ferritin
 --, ILMA 349
 fibrinolysis
 --, acute myocardial infarction 723
 ---, by streptokinase 723
 ----, biochemical parameters 723
 fibronectin
 --, plasma 15
 ---, acute liver failure 15
 ---, liver cirrhosis 15
 flecainid
 --, plasma 389
 --, HPLC 389
 flow-cytometry 935
 fluorimetry
 --, 4-aminobutyric acid 379
 --, cerebrospinal fluid 379
 --, enzymes 189
 foetal development
 --, magnesium 473
 α_1 -foetoprotein 905
 follow-up
 --, thyroid cancer 661
 food
 --, composition 731
 --, creatinine 731
 ---, urine 731
 ---, 3-methylhistidine 731
 ---, urine 731
 --, intake 597
 ---, and catecholamines 597
 ---, and cortisol 597
 ---, and glucose 597
 ---, and insulin 597
 function tests
 --, testing pharmaceuticals 811
- galactose
 --, cataract formation 285
 β -galactosidase
 --, kidney 21
 ---, diabetes mellitus 21
 --, liver 735
 ---, isolation 735
 ---, specificity 735
 --, urine 21
 ---, diabetes mellitus 21
 gallstones
 --, carbohydrates 453
 --, glycoproteins 453
 gammopathy
 --, monoclonal 253
 gas chromatography
 --, carbohydrates 453
 ---, gallstones 453
 --, costs 927
 --, duration 927
 --, hormones 927
 --, analytical performance 927
 --, pharmaceuticals 927
 --, analytical performance 927
 --, phenytoin 773
 --, toxicology 699
- Gc-globulin
 --, isoelectric focusing 545
 --, phenotyping 545
 gel electrophoresis
 --, two dimensional 253
 genetic variants
 --, pseudocholinesterase 671
 gentamycin 905
Gibbs-Helmholtz equation 851
Gibbs potentials
 --, immunoreactions 851
 glomerulonephritis
 --, enzymes 523
 ---, urine 523
 glucocorticoids
 --, receptors 209
 gluconeogenesis
 --, marathon runner 535
 glucose
 --, assay 827
 ---, interferences 827
 --, calibration standard 827
 --, method evaluation 827
 --, plasma 301
 ---, minipig 301
 --, serum 597
 ---, and food intake 597
 glucose-6-phosphate dehydrogenase
 --, bioluminescence assay 129
 α -glucosidase
 --, kidney 21
 ---, diabetes mellitus 21
 --, urine 21
 ---, diabetes mellitus 21
 glutamate dehydrogenase 153
--, myocardial infarction 723
---, fibrinolysis by streptokinase 723
- γ -glutamyltransferase
 --, brush border membrane 449
 --, urine 523
 γ -glutamyltranspeptidase 153
glycation
 --, albumin 223
 --, basement membrane 223
 --, proteins 47
 glycerolphosphate oxidase
 --, triglyceride assay 165
 glycodeoxycholic acid 623
glycoproteins
 --, enzymatic degradation 735
 --, gallstones 453
 glycosaminoglycans
 --, synthesis 527
 --, stimulation by platelet growth factor 527
- granulocytes
 --, elastase 693
 --, function 1
 --, isolation 1
 --, leukocytes 693
 ---, polymorphonuclear 693
 ---, elastase 693
 --, phagocytosis 1
 --, and chemiluminescence 1
 Greiner analyser G 300
 --, urea 195
 growth stimulating factor
 --, platelets 527
 --, isolation 527
 guanosine
 --, assay 175
- haematocrit
 --, blood 301
 --, minipig 301
 haematology
 --, testing pharmaceuticals 811
 haemodialysis
 --, oxalic acid 261
 haemoglobin
 --, glycated 47
 haemolytic disease
 --, haptoglobin 109
 haptens
 --, protein conjugates 337
 haptoglobin
 --, phenotyping 109
 --, diagnostic value 109
 HDL
 --, apolipoprotein A-I 397
 --, cholesterol 113, 397, 515
 --, composition 141
 --, phosphatidyl choline 515
 --, and risk factors of coronary heart disease 515
 hepatitis
 --, fulminant 291
 --, tryptophan, free 291
 ---, plasma 291
 hepatotoxicity
 --, valproic acid 309
 --, metabolites 309
 heteroscedasticity 319
 high performance liquid chromatography see also HPLC
 --, flecainid 389
 --, thiopental 385
 histocompatibility
 --, testing 959
 Hitachi 705
 --, amylases 41
 homocarnosine 379
 hormones
 --, bioassay 927
 --, gas chromatography 927
 --, HPLC 927
 --, immunoassay 927
 hospitalisation
 --, influence 613
 --, on laboratory values 613
 HPLC
 --, hormones 927
 --, pharmaceuticals 927
 --, ribonucleosides 175
 --, minor 175
 hybridoma technology 867
 hydroperoxides
 --, organic 711
 --, lung lavage fluid 711
 α -hydroxybutyrate dehydrogenase
 --, assay 559
 --, drug interference 559
 --, myocardial infarction 723
 --, fibrinolysis by streptokinase 723
- 3-hydroxybutyrate dehydrogenase
 --, bioluminescence assay 129
 hydroxymethylfurfural 47
 17-hydroxyprogesterone
 --, blood 371
 --, plasma 371
 hydroxyproline
 --, total 123
 --, serum 123

- hyperglycaemia
 –, rat 21
 hyperlipaemia
 –, lipoprotein composition 141
 hyperparathyroidism
 –, analyte pattern 319
 ibuprofen
 –, interference 559
 ––, enzyme assays 559
 IgG
 –, synthesis 483
 ––, by lymphocytes 483
 ––, cerebrospinal fluid 483
 ––, multiple sclerosis 483
 ––, non-inflammatory diseases 483
 ILMA 349, 905
 ILSA 349, 905
 immunoadsorption
 –, enzymes 943
 immunoassay
 –, costs 927
 –, duration 927
 –, enzyme- 895
 –, enzymes 943
 –, hormones 927
 ––, analytical performance 927
 –, luminescence 337, 349, 905
 –, macro solid phase 349
 –, particle counting 919
 –, peptides 927
 ––, analytical performance 927
 –, pharmaceuticals 927
 ––, analytical performance 927
 –, phenytoin 773
 –, phosphatase, alkaline, placental 467
 –, proteins 927
 analytical performance 927
 –, radio- 883
 –, solid phase 337
 immunodiffusion
 –, radial 109, 919
 ––, haptoglobin 109
 immuno-enzymometric assay 895
 immunoglobulins
 –, interference 759
 ––, digoxin assay 759
 immunohistochemistry
 –, procedures 953
 immunoinhibition
 –, enzymes 943
 immunonephelometry
 –, α_2 -macroglobulin 633
 –, α_1 -proteinase inhibitor 633
 immunoprecipitation
 –, enzymes 943
 indometacin
 –, interference 559
 ––, enzyme assays 559
 infarction
 –, acute myocardial 723
 ––, fibrinolysis by streptokinase 723
 ––, biochemical parameters 723
 inflammatory diseases
 –, sialic acid 647
 –, serum 647
 influence factor
 –, biological 65
 ––, alcohol 65
 influences
 –, on laboratory values 613
 ––, age 613
 ––, hospitalisation 613
 ––, sex 613
 infrared spectrometry
 –, dimethadione 641
 –, trimethadione 641
 inhibitor
 –, blastogenesis 209
 ––, 17β -carboxamide steroids 209
 –, proteinase 633, 653
 –, α_1 -proteinase 693
 inosine
 –, assay 175
 instrumentation
 –, toxicology 699
 insulin
 –, serum 597
 ––, and food intake 597
 interconversion
 –, 3-oxo- 5α -steroid Δ^4 -oxidoreductase 705
 –, liver 705
 ––, rat 705
 interferences 817
 –, α -amylase assay 489, 677
 –, analgesics 559
 ––, enzyme assays 559
 –, analytical 271, 275
 ––, evaluation 275
 –, antirheumatics 559
 ––, enzyme assays 559
 –, glucose assay 827
 –, immunoglobulins 759
 ––, enzyme immunoassay 759
 ––, digoxin 759
 –, ions 419
 ––, SG test strip 419
 –, rheumatoid factors 759
 ––, enzyme immunoassay 759
 ––, digoxin 759
 –, triglyceride assay 165
 –, uraemia 773
 ––, phenytoin assay 773
 interpretation
 –, computer assisted 407
 ––, electrophoresis 407
 intestine
 –, enzymes 449
 –, perfusion 449
 intracellular pH 641
 iodination
 –, thyroglobulin 661
 iotalamate
 –, and alanine aminopeptidase excretion 787
 ioxaglate
 –, and alanine aminopeptidase excretion 787
 IRMA 905
 isoamylase
 –, serum 41
 ––, *p*-nitrophenyl- α -D-maltoheptaoside 41
 isoelectric focusing
 –, Gc-globulin 545
 isoelectric focusing
 –, vitamin D-binding protein 545
 isoenzymes
 –, α -amylase 427
 –, aspartate aminotransferase 153
 ––, serum 153
 ––, liver diseases 153
 –, creatine kinase 603, 723, 751
 isoluminol 905
 isotope dilution
 –, oestradiol- 17β 551
 ketoprofen
 –, interference 559
 ––, enzyme assays 559
 kidney
 –, diseases 523, 633
 ––, enzymes 523
 ––, urine 523
 ––, proteinase inhibitors 633
 ––, serum 633
 –, enzymes 129
 ––, nephron
 –, failure 61
 ––, myoglobinuric 61
 –, parathyrin extraction 479
 –, rat 21
 ––, glycosidases 21
 ––, diabetes mellitus 21
 –, transplants 523
 ––, enzymes 523
 ––, urine 523
 Kirchhoff equation 851
 kits
 –, diagnostic 817, 827
 ––, evaluation 817, 827
 Kupffer cells 219
 kurtosis
 –, definition 97
 labelling
 –, reagent package 573
 laboratory values
 –, assessment 613
 –, evaluation 613
 –, variations 613
 lactate dehydrogenase
 –, assay 559
 ––, drug interference 559
 –, myocardial infarction 723
 ––, fibrinolysis by streptokinase 723
 laser nephelometry
 –, apolipoproteins 113
 lavage fluid
 –, lung 711
 ––, hydroperoxides, organic 711
 lens
 –, S-(1,2-dicarboxyethyl)-L-cysteine 285
 –, S-(1,2-dicarboxyethyl)-glutathione 285
 leukocytes
 –, neuraminidase 189
 –, polymorphonuclear 693
 ––, elastase 693
 –, sialidase 189
 LDL
 –, apolipoprotein B 35
 –, cholesterol 35, 113, 781
 ––, method comparison 781
 LDL
 –, composition 141
 –, precipitation 781
 ––, by sulphopolyanions 781
 ligand binding assay
 –, duration 927
 –, fundamental analytical steps 927
 light scattering 919
 likelihood quotient 229
 linear regression 431
 lipase
 –, serum 357
 ––, titrimetric assay 357
 ––, effect of temperature 357
 lipids
 –, Niemann-Pick's disease 199
 –, peroxidation 711
 lipoprotein (a) 591
 lipoproteins see also HDL, LDL, VLDL
 –, constituents 35
 –, fractions 141
 ––, composition 141
 ––, in health 141
 ––, in hyperlipaemics 141
 –, serum 113
 ––, constituents 113
 lithocholic acid 623
 liver
 –, acute failure 15
 ––, factor VIII-related antigen 15
 ––, plasma 15
 ––, fibronectin 15
 ––, plasma 15
 –, cirrhosis 15, 147, 291, 319
 ––, analyte pattern 319
 ––, factor VIII-related antigen 15
 ––, plasma 15
 ––, fibronectin 15
 ––, plasma 15
 ––, β_2 -microglobulin 147
 ––, plasma 147
 ––, production 147
 ––, tryptophan, free 291
 ––, plasma 291
 –, diseases 153, 633
 ––, aspartate aminotransferase 153
 ––, isoenzymes 153
 ––, serum 153
 ––, proteinase inhibitors 633
 ––, liver 633
 –, β -galactosidase 735
 ––, isolation 735
 ––, specificity 735
 –, lipids 199
 ––, Niemann-Pick's disease 199
 –, parathyrin extraction 479
 –, rat 705
 ––, 3-oxo- 5α -steroid Δ^4 -oxidoreductase 705
 ––, interconversion 705
 Loewe, Walter Siegfried (1884–1963) 505
 longitudinal evaluation
 –, laboratory values 613
 long term study
 –, plasma constituents 97
 ––, rat 97

- Lp(a) 591
 luciferase 129
 lucigenin 1
 luminescence 337, 349
 –, immunoassay 905
 –, measurement 905
 luminol 1, 337, 905
 luminometers 905
 lung
 –, alveolar surfactant 711
 –, lavage fluid 711
 –, hydroperoxides, organic 711
 lymphocytes
 –, blastogenesis 209
 –, cerebrospinal fluid 483
 –, IgG synthesis 483
 –, multiple sclerosis 483
 –, non-inflammatory diseases 483
 –, differentiation 867
 –, antigens 867
 –, surface antigens 959
 lysophosphatidylcholine
 –, liver 199
 –, spleen 199
 lysophosphatidylethanolamine
 –, liver 199
 –, spleen 199
- α_2 -macroglobulin
 –, assay 633
 –, serum 633
 –, multiple sclerosis 653
 macrophage 219
 magnesium
 –, erythrocytes 717
 –, physical exercise 717
 –, foetal development 473
 –, metabolism 473
 –, plasma 301, 717
 –, minipig 301
 –, physical exercise 717
 –, supplementation 717
 –, in physical exercise 717
 –, and cortisol 717
 –, and electrolytes 717
 –, sweat 717
 –, physical exercise 717
 –, urine 717
 –, physical exercise 717
 marathon runner
 –, amino acid metabolism 535
 –, gluconeogenesis 535
 marker
 –, tumour 969
 mass density
 –, urine 419
 mass spectra
 –, valproic acid 309
 –, metabolites 309
 mass spectrometry
 –, oestradiol-17 β 551
 –, toxicology 699
 matrix
 –, influence 305
 –, albumin assay 305
 –, by bromocresol green 305
 –, serum 751
 –, creatine kinase MB 751
 measles
 –, antibodies 653
 –, multiple sclerosis 653
- membrane
 –, protein 281
 –, abnormality 281
 metabolism
 –, magnesium 473
 –, parathyrin 479
 –, valproic acid 309
 metanephrite
 –, radioimmunoassay 741
 metastases
 –, diagnosis 969
 method comparison
 –, α -amylase 677
 –, catecholamines 539
 –, cholesterol 245
 –, LDL 781
 –, creatine kinase MB 603, 751
 –, phenytoin 773
 –, regression procedures 431
 –, statistical problems 265
 method evaluation
 –, glucose 827
 methods
 –, recommended 811
 –, testing pharmaceuticals 811
 3-methoxy-4-hydroxyphenylethyleneglycol 741
 –, radioimmunoassay 741
 3-methoxytyramine
 –, radioimmunoassay 741
 N1-methyladenosine
 –, assay 175
 N6-methyladenosine
 –, assay 175
 3-O-methyldopamine
 –, antigen preparation 741
 N1-methylguanosine
 –, assay 175
 N2-methylguanosine
 –, assay 175
 3-methylhistidine
 –, meat 731
 –, urine 731
 –, and food composition 731
 N1-methylinosine
 –, assay 175
 methyl palmitate
 –, reticuloendothelial depression 219
 methylumbelliferyl-N-acetylneuraminic acid 189
 Michaelis constant
 –, β -galactosidase 735
 –, liver 735
 microdissection
 –, nephron 129
 β_2 -microglobulin
 –, plasma 147
 –, liver cirrhosis 147
 –, production 147
 –, liver cirrhosis 147
 minerals
 –, plasma 97
 –, rat 97
 minipig
 –, blood constituents 301
 –, reference values 301
 mitogenesis test 505
 model reactions
 –, monovalent 851
 –, polyvalent 851
 molar lineic absorbance see also absorbance 489
- monitoring
 –, drug 271
 –, tumour 969
 multicentre study
 –, α -amylase 677
 –, cholesterol 245
 multiple sclerosis
 –, α_2 -macroglobulin 653
 –, measles antibodies 653
 –, plasminogen 653
 –, proteinase inhibitors 653
 –, IgG synthesis 483
 –, by lymphocytes 483
 –, cerebrospinal fluid 483
 Multistix SG 419
 multivariate decision limits
 –, discrimination of populations 791
 mutants
 –, apolipoprotein A-I 585
 myocardial infarction 723
 –, creatine kinase-MB 603
 –, proteinase inhibitors 633
 –, serum 633
 myoglobin
 –, myocardial infarction 723
 –, fibrinolysis by streptokinase 723
 –, urine 61
 radioimmunoassay 61
- nandrolone
 –, plasma 29
 –, radioimmunoassay 29
 –, serum 29
 –, radioimmunoassay 29
 nephelometric inhibition method 919
 nephelometry 919
 nephron
 –, enzymes 129
 –, microdissection 129
 nephropathy
 –, diabetic 21
 –, rat 21
 nephrotoxicity
 –, contrast media 787
 –, and alanine aminopeptidase excretion 787
 neuraminidase
 –, leukocytes 189
 newborns
 –, bilirubin 609
Niemann-Pick's disease
 –, lipids 199
 4-nitrophenol
 –, dissociation curve 489
 p-nitrophenylheptaoside
 –, substrate 677
 –, α -amylase 677
 p-nitrophenyl-maltoheptaoside
 –, α -amylase substrate 427
 non-inflammatory CNS diseases
 –, IgG synthesis 483
 –, by lymphocytes 483
 –, cerebrospinal fluid 483
 non-parametric analysis 265
 noradrenaline 539
 norepinephrine
 –, plasma 597
 normetanephrine
 –, radioimmunoassay 741
- nortestosterone
 –, plasma 29
 –, radioimmunoassay 29
 –, serum 29
 –, radioimmunoassay 29
- oestradiol
 –, blood 371
 –, plasma 371
 oestradiol-17 β
 –, definitive method 551
 –, isotope dilution 551
 –, mass spectrometry 551
 oestrogens
 –, detection methods 505
 –, in plants 505
 oestrone
 –, blood 371
 –, plasma 371
 opsonization 1
 ornithine carbamyltransferase 153
 osmolality
 –, urine 419
 –, test strip 419
 osmolarity
 –, plasma 301
 –, minipig 301
 oxalic acid
 –, haemodialysis 261
 –, plasma 261
 oxidase
 –, glycerolphosphate 165
 3-oxo-5 α -steroid Δ^4 -oxidoreductase 705
 –, interconversion 705
 –, liver 705
 –, rat 705
 11-oxotestosterone
 –, plasma 461
 –, radioimmunoassay 461
 oxygen
 –, reduction 1
 –, during phagocytosis 1
- PACIA 919
Page's disease
 –, hydroxyproline 123
 –, serum 123
 parameter
 –, combination 791
 paraproteins
 –, serum 53
 –, characterization 53
 parathyrin
 –, carboxylterminal 479
 –, radioimmunoassay 479
 –, metabolism 479
 particle counting immunoassay 919
 pCO
 –, blood 301
 –, minipig 301
 peptides
 –, immunoassay 927
 performance
 –, analytical 573, 817, 827
 –, diagnostic reagent sets 573
 –, evaluation 817, 827
 perfusion
 –, intestine 449
 peroxidation
 –, lipids 711

- peroxides
 –, lung lavage fluid 711
 PGLIA 895
 pH
 –, blood 301
 ––, minipig 301
 –, intracellular 641
 pH-stat method
 –, adenosine deaminase 769
 –, principle 769
 phagocytosis
 –, by granulocytes 1
 ––, chemiluminescence 1
 pharmaceuticals
 –, gas chromatography 927
 –, HPLC 927
 –, immunoassay 927
 –, testing 811
 ––, clinical chemical tests 811
 phenacetin
 –, interference 559
 ––, enzyme assays 559
 phenobarbital
 –, interference 559
 ––, enzyme assays 559
 phenotyping
 –, Gc-globulin 545
 –, haptoglobin 109
 –, vitamin D-binding protein 545
 phenytoin
 –, gas chromatography 773
 –, immunoassay 773
 –, interference 773
 –, uraemia 773
 –, method comparison 773
 phosphatase
 –, acid 331
 ––, serum 331
 –, alkaline 449, 467, 523, 559
 ––, assay 559
 –––, drug interference 559
 ––, brush border membrane 449
 ––, placental 467
 –––, serum 467
 –––, tumour tissue 467
 ––, urine 523
 phosphate, inorganic
 –, plasma 301
 ––, minipig 301
 phosphatidyl choline
 –, HDL 515
 ––, and risk factors of coronary heart disease 515
 –, liver 199
 –, lysosomes 199
 –, spleen 199
 phosphatidylethanolamine
 –, liver 199
 –, lysosomes 199
 –, spleen 199
 phosphatidylinositol
 –, liver 199
 –, lysosomes 199
 –, spleen 199
 phosphatidylserine
 –, liver 199
 –, lysosomes 199
 –, spleen 199
 phospholipids
 –, liver 199
 ––, *Niemann-Pick's* disease 199
 phospholipids
 –, spleen 199
 ––, *Niemann-Pick's* disease 199
 phosphorescence 905
 phosphotungstic acid 35
Planck effectivity quantum 851
 plants
 –, oestrogens 505
 plasma
 –, aldosterone 717
 ––, physical exercise 717
 –, analytes 723
 ––, myocardial infarction 723
 –––, fibrinolysis by streptokinase 723
 –, calcium 717
 ––, physical exercise 717
 –, catecholamines 539, 597
 ––, method comparison 539
 –, cholesterol 245
 –, constituents 97, 301
 ––, minipigs 301
 –––, reference values 301
 ––, variance 97
 ––, rat 97
 –, cortisol 597, 717
 ––, physical exercise 717
 –, dopamine 597
 –, enzymes 723
 ––, myocardial infarction 723
 –––, fibrinolysis by streptokinase 723
 –, epinephrine 597
 –, factor VIII-related antigen 15
 ––, acute liver failure 15
 ––, liver cirrhosis 15
 –, fibronectin 15
 ––, acute liver failure 15
 ––, liver cirrhosis 15
 –, flecainid 389
 ––, HPLC 389
 –, magnesium 717
 ––, physical exercise 717
 –, proteinase inhibitors 653
 –, β_2 -microglobulin 147
 ––, liver cirrhosis 147
 –, nandrolone 29
 ––, radioimmunoassay 29
 –, norepinephrine 597
 –, nortestosterone 29
 ––, radioimmunoassay 29
 –, oxalic acid 261
 –, 11-oxotestosterone 461
 ––, radioimmunoassay 461
 –, potassium 717
 ––, physical exercise 717
 –, proteinase inhibitors 653
 –, proteins, total 653
 –, sodium 717
 ––, physical exercise 717
 –, steroids 371
 ––, influence of storage 371
 –, tryptophan, free 291
 ––, hepatitis, fulminant 291
 ––, liver cirrhosis 291
 –, valproic acid 309
 ––, metabolites 309
 plasminogen
 –, multiple sclerosis 653
 platelets
 –, growth stimulating factor 527
 platelets
 –, growth stimulating factor
 ––, isolation 527
 PMN-elastase
 –, assay 693
 potassium
 –, plasma 301, 717
 ––, minipig 301
 ––, physical exercise 717
 –, sweat 717
 ––, physical exercise 717
 –, urine 717
 ––, physical exercise 717
 practicability
 –, diagnostic reagent sets 573
 precision
 –, radioimmunoassay 883
 predictive value 229
 –, tumour markers 969
 principal compound procedures 431
 probability theory 791
 procollagen type III
 –, propeptide 237
 ––, aminoterminal 237
 ––, CSF 237
 product information 573
 production
 –, β_2 -microglobulin 147
 ––, liver cirrhosis 147
 –, reference values 203
 prognosis
 –, tumour 969
 prostate
 –, cancer 331
 protein
 –, abnormal 281
 ––, erythrocyte membrane 281
 –––, pseudohypoparathyroidism type 1 281
 –, immunoassay 927
 –, mapping 253
 –, total 301, 653
 ––, plasma 301
 –––, minipig 301
 –––, multiple sclerosis 653
 protein kinase 705
 proteins
 –, electrophoresis 407
 ––, interpretation, computer assisted 407
 –, silver staining 53
 proteinase inhibitor
 –, multiple sclerosis 653
 α_1 -proteinase inhibitor
 –, assay 633
 ––, serum 633
 –, elastase complex 693
 –, multiple sclerosis 653
 pseudocholinesterase
 –, genetic variants 671
 –, serum 671
 ––, continuous colorimetric assay 671
 pseudohypoparathyroidism
 –, type 1 281
 ––, protein abnormality 281
 –––, erythrocyte membrane 281
 pseudouridine
 –, assay 175
 pyelonephritis
 –, enzymes 523
 ––, urine 523
 quality
 –, analytical 883
 radial immunodiffusion 919
 radioimmunoassay
 –, application 883
 –, automatisation 883
 –, calmodulin 185
 –, catecholamines 741
 –, detection limit 883
 –, developmental trends 883
 –, digoxin 119, 403
 ––, urine 403
 –, enzymes 943
 –, history 883
 –, instrumentation 883
 –, myoglobin 61
 –, nandrolone 29
 –, nortestosterone 29
 –, parathyrin 479
 ––, carboxyterminal 479
 –, principles 883
 –, propeptide 237
 ––, procollagen type III 237
 –, quality, analytical 883
 –, reliability 883
 –, sensitivity 61
 ––, definition 61
 –, separation methods 883
 –, substances assayable 883
 –, thyroglobulin 661
 rat
 –, diabetes mellitus 21
 –, liver 705
 ––, 3-oxo-5 α -steroid Δ^4 -oxidoreductase 705
 –––, interconversion 705
 –, plasma constituents 97
 reaction
 –, energies 851
 –, model 851
 ––, monovalent 851
 ––, polyvalent 851
 reaction kinetics 851
 reaction rate constants 851
 reactive equilibrium constants 851
 reagent plate
 –, ammonia 105
 reagent sets 817, 827
 receiver operating characteristic analysis 229
 receptors
 –, glucocorticoid 209
 reference interval
 –, analytes 65
 –, appropriate use 613
 reference materials 573, 817, 827
 reference range
 –, alanine aminopeptidase 787
 ––, urine 787
 –––, children 787
 –, blood constituents 301
 –, children 301
 –, elastase 693
 –, evaluation 319
 reference values
 –, blood constituents 301
 ––, minipig 301
 –, production 203
 reflectometer
 –, blood ammonia 105

- regression analysis 265
 regression procedures
 -, method comparison 431
 reliability
 -, radioimmunoassay 883
 renal disease
 -, proteinase inhibitors 633
 --, serum 633
 rheumatoid factors
 -, interference 759
 --, digoxin assay 759
 RIA 905
 ribonucleosides
 -, minor 175
 --, HPLC assay 175
 ---, serum 175
 ---, urine 175
 risk factors
 -, coronary heart disease 515, 591
 sample size
 -, determination 431
 sandwich assay 895
Scatchard plot 883
 screening
 -, tumour 969
 selection
 -, diagnostic reagent sets 573
 -, individuals 203
 --, for reference values 203
 sensitivity
 -, diagnostic 79, 229, 969
 --, tumour markers 969
 -, radioimmunoassay 61
 --, definition 61
 serum
 -, albumin 305, 685
 --, bromocresol green 305
 --, bromocresol purple 685
 -, amylase 41
 --, *p*-nitrophenyl- α -D-maltoheptaoside 41
 -, α -amylase 427, 489, 677
 --, 2-chloro-4-nitrophenyl- β -D-maltoheptaoside 489
 --, *p*-nitrophenyl-maltoheptaoside 427
 ---, action pattern 427
 -, aspartate aminotransferase 153
 --, isoenzymes 153
 ---, liver diseases 153
 -, cholesterol 245
 -, constituents 811
 --, testing pharmaceuticals 811
 -, digoxin 119
 --, radioimmunoassay 119
 -, enzymes 559
 --, interferences 559
 -, glucose 597
 -, HDL apolipoprotein A-I 397
 -, HDL cholesterol 397
 -, hydroxyproline 123
 --, total 123
 -, insulin 597
 -, isoamylase 41
 --, *p*-nitrophenyl- α -D-maltoheptaoside 41
 -, lipase 357
 --, titrimetric assay 357
 ---, effect of temperature 357
 serum
 -, lipoproteins 113
 --, constituents 113
 -, α_2 -macroglobulin 633
 -, matrix 751
 --, creatine kinase MB 751
 -, nandrolone 29
 --, radioimmunoassay 29
 -, nortestosterone 29
 --, radioimmunoassay 29
 -, paraproteins 53
 --, characterization 53
 -, phenytoin 773
 --, gas chromatography 773
 --, immunoassay 773
 -, phosphatase 331, 467
 --, acid 331
 --, alkaline 467
 --, placental 467
 -, proteinase inhibitor 653
 -, α_1 -proteinase inhibitor 633
 -, pseudocholinesterase 671
 -, ribonucleosides 175
 --, minor 175
 --, HPLC assay 175
 -, sialic acid 647
 --, cancer 647
 --, inflammatory diseases 647
 -, thiopental 385
 --, HPLC 385
 -, thyroglobulin 661
 --, thyroid carcinoma 661
 -, triglycerides 165
 -, VLDL 35
 --, precipitation 35
 sex dependence
 -, laboratory values 613
 sex hormones 505
 sex hormones binding globulin 371
 SG test strip 419
 sialic acid
 -, serum 647
 --, cancer 647
 --, inflammatory diseases 647
 sialidase
 -, leukocytes 189
 sialidosis 189
 silver staining
 -, proteins 53, 253
Sips-Hill-Nerst equation 851
 skewness
 -, definition 97
 smokers
 -, carboxyhaemoglobin 229
 -, CO 229
 sodium
 -, plasma 301, 717
 --, minipig 301
 --, physical exercise 717
 -, sweat 717
 --, physical exercise 717
 -, urine 717
 --, physical exercise 717
 solid phase immunoassay 337 349
Southern blot 394
 SPALT 349, 905
 specificity
 -, diagnostic 79, 229, 969
 --, tumour markers 969
 spectrometers
 -, specifications 565
 --, listing 565
 sphingomyelin
 -, liver 199
 -, spleen 199
 spleen
 -, lipids 199
 --, *Niemann-Pick's* disease 199
 staging
 -, tumour 969
 standard
 -, glucose 827
 standard bicarbonate
 -, blood 301
 --, minipig 301
 standardisation
 -, albumin 685
 --, bromocresol purple 685
 standardised principal components analysis 265
 statistics
 -, problems 265
 --, in method comparisons 265
 steroids
 -, blood 371
 --, influence of storage 371
 -, chromatography 29
 -, plasma 371
 --, influence of storage 371
 stomach carcinoma
 -, phosphatase, alkaline 467
 --, placental 467
 storage
 -, blood 371
 --, steroid assay 371
 -, plasma 371
 --, steroid assay 371
 streptokinase
 -, fibrinolysis 723
 --, in myocardial infarction 723
 --, biochemical parameters 723
 streptozotocin 21
 substrate
 -, chromogenic 633
 3 α -sulfolithocholic acid 623
 surfactant
 -, alveolar 711
 --, hydroperoxides, organic 711
 survey
 -, bilirubin 609
 --, neonatal 609
 sweat
 -, calcium 717
 --, physical exercise 717
 -, magnesium 717
 --, physical exercise 717
 -, potassium 717
 --, physical exercise 717
 -, sodium 717
 --, physical exercise 717
 SWFIA 895
 synephrine
 -, radioimmunoassay 741
 T cell
 -, monitoring 959
 -, monoclonal antibodies 959
 --, subsets 959
 taurocholic acid 623
 technicians
 -, education 497
 --, training 497
 temperature
 -, dependence 357
 --, lipase assay 357
 test strip
 -, osmolality 419
 --, urine 419
 testosterone
 -, blood 371
 -, free 371
 --, blood 371
 --, plasma 371
 -, plasma 371
 therapy
 -, control 47
 --, diabetes mellitus 47
 -, monitoring 215
 --, thyroid carcinoma 215
 thermodynamic functions 851
 thiopental
 -, serum 385
 --, HPLC 385
 β -thromboglobulin 527
 thyroglobulin
 -, serum 661
 --, thyroid carcinoma 661
 -, therapy monitoring 215
 --, thyroid carcinoma 215
 thyroid
 -, carcinoma 215, 661
 --, therapy monitoring 215
 --, thyroglobulin 215, 661
 ---, serum 661
 thyroxine
 -, SPALT 349
 thyroxine binding globulin
 -, CELIA 349
 tissue
 -, antigens 867
 -, typing 959
 titrimetric assay
 -, lipase 357
 --, effect of temperature 357
 toxicology
 -, instrumentation 699
 tracer
 -, luminescent 337
 training
 -, technicians 497
 transformation
 -, Langmuir-Michaelis-Menten 851
 -, Scatchard 851
 -, Sips-Hill-Nerst 851
 transplantation
 -, antigens 959
 trauma
 -, proteinase inhibitors 633
 --, serum 633
 triglycerides
 -, hydrolysis 357
 --, by lipase 357
 ---, activation energy 357
 -, plasma 301
 --, minipig 301
 -, serum 165
 --, glycerolphosphate oxidase 165
 -, VLDL 113
 trimethadione
 -, infrared spectrometry 641
 tryptophan
 -, free 291
 --, plasma 291
 ---, hepatitis, fulminant 291
 ---, liver cirrhosis 291

- tumour
 --, antigens 867
 --, cell 935
 --, CEA antibody 935
 --, DNA 935
 --, identification 935
 --, volume 935
 --, diagnosis 969
 --, marker 647, 969
 --, diagnostic sensitivity 969
 --, diagnostic specificity 969
 --, predictive value 969
 --, sialic acid 647
 ---, serum 647
 --, monitoring 969
 --, prognosis 969
 --, screening 969
 --, staging 969
 --, tissue 467
 --, phosphatase, alkaline 467
 ---, placental 467
 turbidimetry 919
- uraemia
 --, interference 773
 --, phenytoin assay 773
- urea
 --, Greiner G 300 195
 --, myocardial infarction 723
 --, fibrinolysis by streptokinase 723
 --, plasma 301
 --, minipig 301
- uridine
 --, assay 175
 urinary antigens 867
- urine
 --, alanine aminopeptidase 787
 --, and contrast media 787
 --, α -amylase 489, 677
 --, 2-chloro-4-nitrophenyl-
 β -D-maltoheptaoside
 489
 --, calcium 717
 --, physical exercise 717
 --, constituents 811
 --, testing pharmaceuticals
 811
 --, creatinine 731
 --, and food composition
 731
 --, digoxin 403
 --, enzymes 523
 --, multiple forms 523
 --, magnesium 717
 --, physical exercise 717
 --, mass density 419
 --, 3-methylhistidine 731
 --, and food composition 731
 --, myoglobin 61
 --, radioimmunoassay 61
 --, osmolality 419
 --, test strip 419
 --, potassium 717
 --, physical exercise 717
 --, rat 21
- urine
 --, rat
 --, glycosidases 21
 --, diabetes mellitus 21
 --, ribonucleosides 175
 --, minor 175
 --, HPLC assay 175
 --, sodium 717
 --, physical exercise 717
 --, valproic acid 309
 --, metabolites 309
 ursodeoxycholic acid 623
- validity
 --, analytic 229
 --, CO 229
 --, CO-Hb 229
 --, diagnostic 229
 --, CO 229
 --, CO-Hb 229
 valproic acid
 --, hepatotoxicity 309
 --, metabolites 309
 --, hepatotoxicity 309
 --, plasma 309
 --, urine 309
 --, plasma 309
 --, urine 309
 Q₁₀value
 --, lipase 357
van't Hoff equation 851
 variability 817
- variance
 --, components of 97
- variations
 --, analytical 613
 --, biological 613
 --, intra-individual 613
- vitamin D-binding protein
 --, isoelectric focusing 545
- phenotyping 545
- VLDL
 --, cholesterol 113
 --, composition 141
 --, serum 35
 --, precipitation 35
 --, triglycerides 113
- volume
 --, cell 935
 --, tumour 935
- X-ray
 --, contrast media 787
 --, and alanine aminopeptidase excretion 787
- X-transformation 319
- zinc
 --, carbonic anhydrase 159
 --, erythrocytes 159
- zymosan
 --, reticuloendothelial stimulation 1, 219

An Evaluation of Four Different Luminescence Immunoassay Systems: CELIA (chemiluminescent immunoassay), SPALT (solid-phase antigen luminescence technique), ILMA (immunoluminometric assay) and ILSA (immunoluminometric labelled second antibody)

A critical study of macro solid phases for use in immunoassay systems, Part III¹)

By W. G. Wood, H. Fricke, J. Haritz, A. Gadow, Heidi-Susanne Krausz, Bettina Tode, C. J. Strasburger and P. C. Scriba

Klinische Laboratorien, Klinik für Innere Medizin (Direktor: Prof. Dr. P. C. Scriba)
Medizinische Hochschule Lübeck

(Received June 7/December 19, 1983)

Summary: The performance of different solid-phase luminescence immunoassays has been documented using four different assay concepts. These are CELIA (chemiluminescence immunoassay), SPALT (solid-phase antigen luminescence technique), ILMA (immunoluminometric assay) and ILSA (immunoluminometric labelled second-antibody assay). CELIA is analogous to a solid-phase radioimmunoassay and uses a labelled antigen, SPALT and ILSA use a labelled second (species-specific) antibody and ILMA a labelled substance-specific antibody, i. e. analogous to the immunoradiometric assay. Both bioluminescent and chemiluminescent labels have been used. Pyruvate kinase was used for bioluminescence and diazoluminol and N-(4-amino-butyl)-N-ethyl isoluminol hemisuccinamide for chemiluminescence. Relevant quality-control parameters and reference ranges have been given for the optimised assays. Assays described are: thyroxine, thyroxine binding globulin, cortisol, caeruloplasmin, ferritin and C-reactive protein.

Luminescence immunoassays with coefficients of variation comparable with radioimmunoassay have been designed, values of under 5% being obtainable within the working range of the assay.

Beurteilung von vier verschiedenen Lumineszenz-Immunoassays:

CELIA (chemiluminescent immunoassay),
SPALT (solid-phase antigen luminescence technique),
ILMA (immunoluminometric assay) und
ILSA (immunoluminometric labelled second antibody).

Eine kritische Untersuchung von Makro-Festphasen zum Gebrauch in Immunoassay-Systemen, Teil III¹)

Zusammenfassung: Die Entwicklung und Durchführung von Lumineszenzimmunoassays werden am Beispiel von vier verschiedenen Assaykonzepten aufgezeigt. Der CELIA (Chemilumineszenzimmunoassay) verwendet markiertes Antigen, SPALT (Solid-Phase Antigen Luminescence Technique) und ILSA (Immunoluminometric Labelled Second-Antibody Assay) markierten spezies-spezifischen „zweiten“ Antikörper und der ILMA (Immunoluminometric Assay) substanz-spezifischen Antikörper, die markiert sind. Sowohl Biolumineszenz (Pyruvatkinase)- als auch Chemilumineszenz (Diazoluminol und N-(4-Aminobutyl)-N-ethyl-isolu-

¹) Part I: J. Clin. Chem. Clin. Biochem. 21, 789–787. Part II: J. Clin. Chem. Clin. Biochem. 22, 337–347.

minol-hemisuccinamid)-Markierungen wurden verwendet und gegenübergestellt. Qualitätskontrollkenngrößen und Referenzbereiche im Serum werden für die optimierten Assays ermittelt. Es werden Lumineszenzimmunoassays für die folgenden Substanzen beschrieben: Thyroxin, thyroxin-bindendes Globulin, Cortisol, Ferritin, Caeruloplasmin und C-reactives Protein.

Die entwickelten Lumineszenzimmunoassays zeigen dem Radioimmunoassay vergleichbare Variationskoeffizienten mit Werten unter 5% im relevanten Bereich.

Introduction

This third and final part of a study upon solid phases for immunoassay describes the assays which have been developed from the experiments described in the first two parts (1, 2). Both functional and non-functional assay systems have been presented as well as comparisons between different assay systems for the same analyte.

The assays described include those using labelled antigens and labelled first or second antibodies. The labels used are: diazoluminol and N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide, the latter being coupled via an active ester of N-hydroxysuccinamide. The synthesis of the labels has already been described (2). The assays represent different analytes (haptens or peptides) and methods. Where applicable, assays which have already been introduced into the routine laboratory are presented with relevant quality-control parameters and comparisons with the methods which they have replaced.

Materials and Methods

Materials

Antibodies

Antibodies to human liver and spleen ferritins were purchased from Atlanta (Pelfreeze), Heidelberg; Proma (Seward), Augsburg; Boehringer-Ingelheim (DAKO), Ingelheim; these being the distributors in the FRG. Antibodies to human C-reactive protein and human thyroxine binding globulin were obtained from Proma and Boehringer-Ingelheim.

Antibodies to caeruloplasmin were purchased from Behringwerke, Marburg a.d. L., FRG, whereas those for cortisol and thyroxine were donations from Dr. Mario Pazzaglia, Firenze, Italy and the Fa. Henning Berlin GmbH respectively.

Donkey anti-rabbit IgG was purchased from Wellcome Diagnostika, Burgwedel, FRG and rabbit anti-sheep IgG from Boehringer Ingelheim.

Standard materials

Ferritin standards were obtained from Travenol-Clinical Assays, Munich, FRG, C-reactive protein serum standard from Behringwerke, thyroxine and cortisol standards from Henning Berlin and Diagnostic Products Corporation (Hermann Biermann, Bad Nauheim, FRG) respectively. Human transferrin was purchased from Behringwerke, human caeruloplasmin from Serva, Heidelberg, FRG or Sigma, Munich, human thyroxine binding globulin being a gift from Prof. K. Horn and Dr. R. Gärtner, Munich.

Equipment

The luminometers used were either the LKB-1251 (LKB Instruments, Gräfelfing, FRG) or the LB-950 (Laboratorium Prof. Dr. Berthold, Wildbad, FRG). The LKB-1251 was a 25-sample semi-automatic instrument with microprocessor, the LB-950 had a 300 sample capacity and was also microprocessor controlled. Both instruments were at the time of the experiments not able to process data fully so that an off-line data-processing with a desk-top computer (CBM 8032 – Commodore Business Machines, Neu-Isenburg, FRG) and spline function programme was necessary.

Methods

CELIA – chemiluminescent immunoassay

This type of assay is analogous to a solid-phase radioimmunoassay in which the first antibody was coupled to a polystyrene ball (1) and in which the tracer was an antigen labelled with N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide instead of a radioactive marker. Table 1 shows the assay flow sheet for a TBG CELIA.

Tab. 1. Thyroxine binding globulin CELIA flow sheet.

50 µl sample or standard
200 µl assay buffer (0.05 mol/l Tris-HCl containing 2.50 g/l bovine serum albumin, pH 7.4)
1 sheep anti human TBG coated ball
Incubate at ambient temperature for 30 min
50 µl diazoluminol labelled TBG (1:100 dilution*)
Incubate as above and wash with 2 × 1 ml 0.15 mol/l NaCl containing 0.15 ml/l Tween 20.
Transfer balls to measuring cuvettes and load luminometer.

The light initiation step is identical with that shown in table 2.

* The diazotisation was analogous to the method described in I.c. (2), replacing the second antibody with thyroxine binding globulin. The dilution factor given here is the further dilution of the TBG-diazoluminol. The amount of label added to each tube was approximately 100 ng.

ILMA – immunoluminometric assay

The ILMA is analogous to the IRMA (immunoradiometric assay) (3) and is especially suited for assays where the antigen is either unavailable or prohibitively expensive so that a SPALT (see below) assay is out of the question. Several antibody-pairs were tested until a suitable combination was found. Table 2 shows an assay flow sheet for a ferritin ILMA.

ILSA – immunoluminometric labelled second-antibody assay

The ILSA is identical with the ILMA, but with one exception, and that is that a labelled second antibody is used in addition to the two substance-specific antibodies used in the ILMA. This assay was only used in cases where diazoluminol was used for labelling the antibodies, in order to achieve maximal sensitivity. Table 3 shows a flow sheet for a C-reactive protein ILSA.

Tab. 2. Ferritin ILMA flow sheet.

20 µl sample or standard
 200 µl assay buffer (0.025 mol/l phosphate/0.025 mol/l Tris-HCl containing 0.5 ml/l Tween 20 and 1.25 g/l bovine serum albumin, pH 7.4)
 1 goat anti human liver ferritin coated ball
 Incubate for 3 h on a horizontal rotator (180 min⁻¹)
 Wash with 2 × 5 ml 0.15 mol/l NaCl containing 0.15 ml/l Tween 20
 200 µl N-(4-aminobutyl)-N-ethylisoluminol hemisuccinamide labelled rabbit anti human ferritin (1:500 dilution)*
 Incubate and wash as above and transfer balls to measuring cuvettes.
 Add 250 µl 0.15 mol/l NaCl and load luminometer. Initiate light reaction with 1 mol/l NaOH, 2 mg/l microperoxidase-MP 11 and 0.15 mol/l H₂O₂ (100 µl + 10 µl + 360 µl respectively). Integrate the light signal over 20 s

* This represents the dilution of the labelled antibody after coupling to N-(4-aminobutyl)-N-ethylisoluminol hemisuccinamide using the same method for labelling donkey anti rabbit IgG – see I.c. (2).

Tab. 3. C-reactive protein ILSA flow sheet.

10 µl sample or standard, 1:10 dilution in assay buffer (0.05 mol/l Tris-HCl containing 2.5 g/l bovine serum albumin, pH 7.6)
 200 µl assay buffer
 1 sheep anti human C-reactive protein coated ball
 Incubation 60 min at 37 °C in a water bath, followed by 2 × 5 ml wash with assay buffer
 200 µl rabbit anti human C-reactive protein (1:500 dilution)
 Incubate and wash as above
 300 µl diazoluminol labelled donkey anti rabbit serum (1:60 dilution*)
 Incubate as above, wash and transfer balls to measuring cuvette. Load luminometer and proceed as in table 2.

* represents the further dilution of the labelled antibody as prepared in I.c. (2).

SPALT – solid phase antigen luminescence technique

The SPALT principle has been described in detail elsewhere (4, 5), and only the variations are briefly described here. The SPALT assay can be set up as either a competitive or sequential assay, depending upon whether the solid phase antigen is added together with the first antibody and sample or after a pre-incubation of first antibody and sample. Tables 4 and 5 show competitive and sequential SPALT assays for caeruloplasmin and thyroxine respectively.

Assay semi-automation

The assays were originally set up in 55 × 12 mm polystyrene tubes which increased the time needed for pipetting and wash steps as each tube had to be processed separately. To increase throughput and reduce the workload assays were set up in either 20 or 60 well trays (cf. Abbott hepatitis kits). The wash steps were carried out using a Pentawash multiple wash device (Abbott Laboratories) where 5 wells were washed simultaneously with 5 ml wash solution. The antigen-antibody reaction was speeded up by incubating the trays on a horizontal rotator at 180 min⁻¹.

Tab. 4. Caeruloplasmin SPALT flow sheet.

50 µl sample or standard, 1:25 dilution in assay buffer (see table 2)
 150 µl rabbit anti caeruloplasmin (1:500 dilution)
 Incubate at ambient temperature for 10 min*
 1 human caeruloplasmin coated ball
 Incubate for 50 min on horizontal rotator (180 min⁻¹) at ambient temperature
 Wash with 2 × 5 ml 0.15 mol/l NaCl containing 0.15 ml/l Tween 20
 200 µl donkey anti rabbit IgG labelled with N-(4-aminobutyl)-N-ethylisoluminol hemisuccinamide (1:150⁺ dilution)
 Incubate for 60 min on rotator and wash as above. Transfer balls to measuring cuvettes and proceed as in table 2.

* represents dilution of labelled antibody as prepared in I.c. (2).
 * this step improved the precision of the assay.

Tab. 5. Thyroxine SPALT flow sheet.

25 µl sample or standard
 150 µl assay buffer (0.05 mol/l Tris-HCl containing 1.58 mmol/l 8-anilino-1-naphthalene sulphonic acid (ammonium salt), pH 7.5)
 100 µl rabbit anti thyroxine (1:500 dilution)
 Incubate for 60 min at ambient temperature
 1 Transferrin-thyroxine coated polystyrene ball*
 Incubate as above, but on horizontal rotator and wash with 2 × 1 ml wash buffer (0.05 mol/l Tris-HCl containing 0.15 ml/l Tween 20, pH 7.5)
 300 µl donkey anti rabbit IgG labelled with either pyruvate kinase or diazoluminol (1:50 dilution)
 Incubate for 60 min on horizontal rotator and wash with 1 ml wash buffer followed by 1 ml 0.15 mol/l NaCl. Transfer balls to measuring cuvettes and proceed with the light initiation step as in table 2.

* Synthesis of the thyroxine-transferrin conjugate has been described in I.c. (2).

The improvement in precision, shortening of assay time and semi-automation of all methods more than compensated for the additional cost of buying the equipment. Moreover, the trays could be re-used after washing without the precision and accuracy of the assay being influenced.

Results

Comparison of a CELIA and ILMA for thyroxine binding globulin (TBG)

Figure 1 shows standard curves for a TBG-CELIA and a TBG-ILMA. Table 6 shows the relevant assay and quality control data. The antibody bound to the solid phase was the same in each case as was the label used, in this case diazoluminol. The TBG used for labelling was identical with that used for making up the standards in both assays.

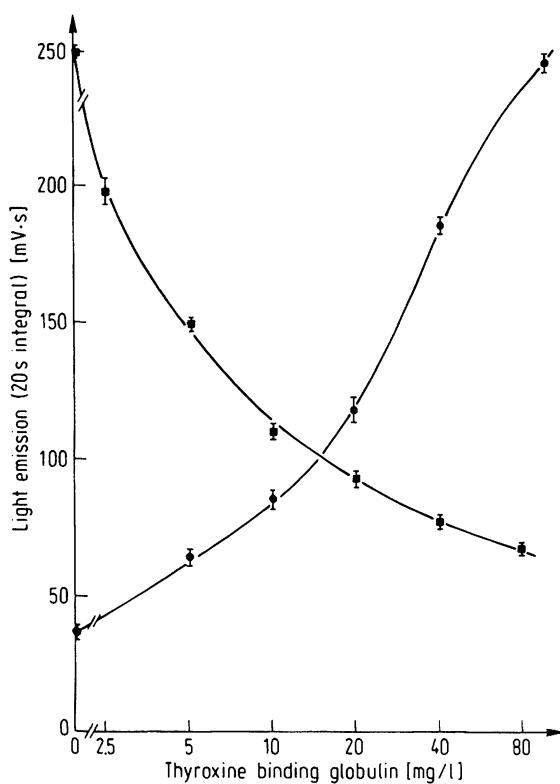


Fig. 1. Comparison between the thyroxine binding globulin CELIA (■—■) and ILMA (●—●). Both assays were measured on an LKB 1251 luminometer, the ordinate representing the integral of the light curve over 20 seconds. Each standard curve point is shown with the mean and 2 standard deviation (95% confidence-) limits.

Comparison between labelling using ILMA and ILSA for ferritin as examples

Figure 2 shows three standard curves using identical starting reagents. For the ILSA the second antibody (donkey anti-rabbit IgG) was labelled with diazoluminol (2), for the ILMAs both diazoluminol and N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide were used to label the second anti-ferritin antibody. Table 7 shows relevant data from all three curves, here with special reference to the sensitivity (lowest detectable antigen level).

Comparison of different pH values to initiate the light reaction using a serum cortisol SPALT as an example

Table 8 shows a comparison between three cortisol SPALT assays set up at the same time with the same reagents. The difference between the assays is that one is oxidised at pH 8.6 to initiate the light reaction, the second with sodium hydroxide, directly after addition, and the third, after the solid phase has been left in contact with sodium hydroxide for 2 h. The assay flow sheet up until the light-reaction step is shown in table 9.

Tab. 6. Comparison of thyroxine binding globulin (TBG) CELIA and ILMA using diazoluminol as label.

Parameter	Assay 1 ⁺	Assay 2
Assay type	CELIA	ILMA
Sample size (μ l)	50	1 (20 μ l 1:20 dilution)
Standard matrix	Buffer	Buffer
Standard curve		
<i>Counts</i> ⁺⁺		
Zero standard (B_0)	250	37
5 mg/l standard (B_5)	150	65
80 mg/l standard (B_{80})	67	245
<i>Ratios</i>		
B_0/B_{80}	3.73*	0.151
B_5/B_0	0.60	1.76
B_{80}/B_0	0.268	6.62*
<i>Quality control</i>		
Control sera (mg/l)**		
H1 (14 ± 3) (mean \pm s.d.)	above 80	13.6
H2 (26 ± 5)	above 80	27.3
H3 (37 ± 6)	above 80	35.9
<i>Correlation data***</i>		
No. of samples	—	89
Correlation coefficient r	—	0.985
Intercept a_{yx} (mg/l)	—	-2.74
Slope b_{yx}	—	0.976
Range of values used (mg/l)	—	10–43

⁺ Both assays were performed simultaneously.

⁺⁺ Expressed as mV · 20 s (integral)

* These values represent the dynamic range for the CELIA and ILMA respectively.

** The CELIA, although giving a standard curve, was unable to measure serum samples, and was therefore abandoned. Target values in brackets.

*** The correlation coefficient and related data was determined from a comparison with the Henning TBG-RIA, results from 6 assays being used. The RIA values were entered as x .

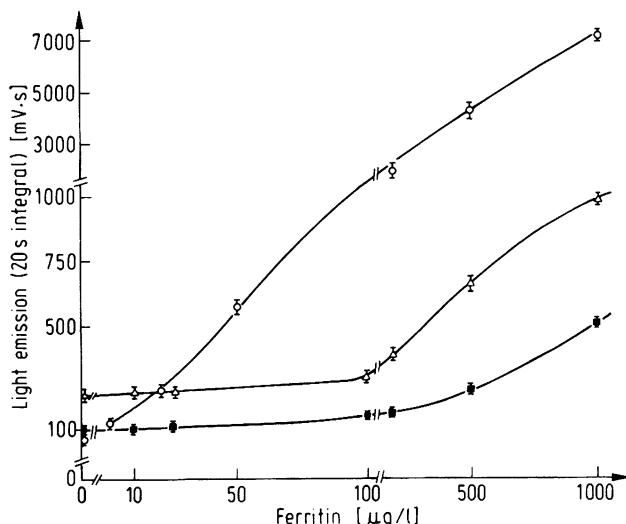


Fig. 2. Comparison of three ferritin assays using diazoluminol (Δ — Δ ILSA; ■—■ ILMA) and N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide (\circ — \circ ILMA) labelled antibodies. Please note that the scales are not linear. The symbols and their significance are as in figure 1.

Tab. 7. Comparison of ferritin ILMA and ILSA using diazoluminol and N-(4-aminobutyl)-N-ethylisoluminol hemisuccinamide (ABEI-H) as labels – relevant assay data.

Parameter		ILMA-1	ILMA-2	ILSA
	Label	Diazo-luminol	ABEI-H	Diazo-luminol
Counts⁺				
Zero standard (B_0)		103	78	222
5 µg/l standard (B_5)		–	125	–
10 µg/l standard (B_{10})		108	–	238
200 µg/l standard (B_{200})		155	1940	370
1000 µg/l standard (B_{1000})		507	4210	965
Ratios of counts				
B_5/B_0		–	1.60	–
B_{10}/B_0		1.05	–	1.07
B_{200}/B_0		1.50	24.9	1.67
B_{1000}/B_0 ⁺⁺		4.92	54.0	4.35
Spread of counts^{**}				
$B_{1000} - B_0$		404	4132	743
Sample size (µl)		100	20	100
Assay time (h)		24	6	26
Control serum values (µg/l)**				
D4 – target value 16 ± 1.9		30	16.4	19.0
D5 – target value 53 ± 4.2		55.0	48.3	52.4
D6 – target value 180 ± 6		192	164	177

⁺ Integral over 20 s, given in 1000 "Berthold light units"

⁺⁺ Expression of the dynamic range of the assay

* Represents the actual spread of counts between the lowest and highest standard.

** Values given as mean \pm 1 standard deviation. The values given are the mean of duplicate values.

Tab. 8. Effect of pH and exposure time to sodium hydroxide on the light emission using the cortisol SPALT as an example.

Parameter	pH 8 ⁺	pH 13 ⁺	pH 13 ⁺ immediate after 2 h
Light emission of zero standard (B_0)	3294*	5391	20444
Light emission of unspecific binding (UB)	85*	103	441
Light emission of 2650 nmol/l standard (S_{2650})	837*	1385	6726
Ratio UB/ B_0	0.03	0.02	0.02
Ratio S_{2650}/B_0	0.25	0.26	0.33
50% intercept (nmol/l)	660	473	908
Control serum D4 (nmol/l) ⁺⁺	154	132	143
Control serum D5	622	638	539
Control serum D6	1523	1413	1721

* Results in 1000 "Berthold Light Units"

+ All assays were set up at the same time. The results in column 2 were obtained when the tubes were processed directly after NaOH addition, those in column 3 when the light initiation step took place 2 h after NaOH addition. The results in column 1 were obtained when 0.5 mol/l phosphate buffer replaced the 1 mol/l NaOH.

++ Results expressed are the mean of duplicate tubes.

Tab. 9. Cortisol SPALT flow sheet.

10 µl sample or standard
200 µl rabbit anti cortisol, 1:4000 in assay buffer (0.1 mol/l phosphate containing 0.1 mol/l sodium salicylate, pH 7.5)
1 cortisol-3-carboxymethyloxime-ovalbumin coated ball
Incubate on horizontal rotator (180 min ⁻¹) for 35 min at ambient temperature
Wash with 2 × 5 ml 0.15 mol/l NaCl containing 0.15 ml/l Tween 20
200 µl N-(4-aminobutyl)-N-ethylisoluminol hemisuccinamide labelled donkey anti rabbit IgG (1:180 dilution*)
Incubate as above, but for 45 min, wash as above and proceed as described in table 2 for the ball-transfer and light-initiating steps

* See table 4.

Comparison between pyruvate kinase and diazoluminol as label for the second antibody using a thyroxine SPALT as an example

The assay flow scheme has already been shown in table 5. Figure 3 shows standard curves for both assays, the relevant assay data being shown in table 10.

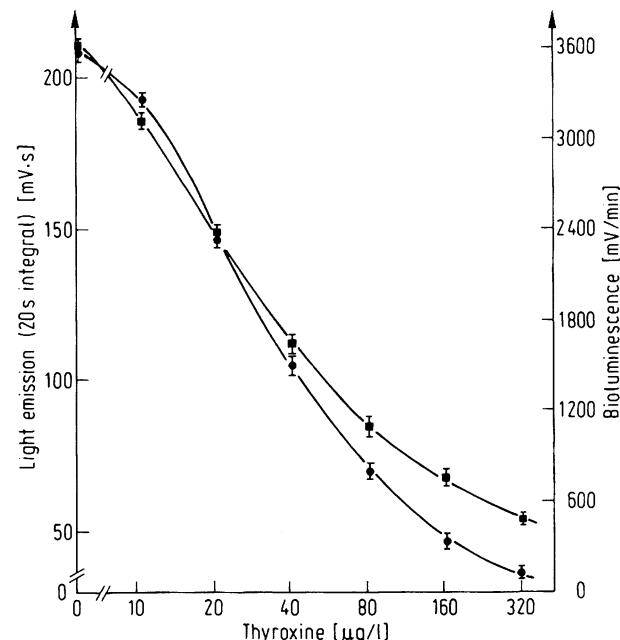


Fig. 3. Comparison of use of a bioluminescent (pyruvate kinase ■—■) label and a chemiluminescent label in a thyroxine SPALT. Both assays were measured on an LKB 1250 luminometer, the left-hand ordinate showing the chemiluminescent signal as 20 s integral, the right-hand ordinate the slope of the ATP-generation curve, expressed as mV/min.

Tab. 10. Comparison between a chemiluminescent and bioluminescent labelled SPALT assay for serum thyroxine.

Parameter		Assay 1*	Assay 2
	Label	Diazoluminol	Pyruvate kinase
Standard curve			
<i>Counts</i>			
Zero standard (B_0)		240	3780
12 nmol/l standard (B_{12})		222	3280
410 nmol/l standard (B_{410})		66	674
Unspecific binding (UB)		31	202
<i>Ratios</i>			
UB/B_0		0.130	0.053
B_{12}/B_0		0.925	0.868
B_{410}/B_0		0.275	0.178
B_0/B_{410}^{++}		3.64	5.61
<i>Intercepts (nmol/l)</i>			
80%		21.4	23.4
50%		64.8	57.4
20%		313	285
Quality control			
Serum A (27 ± 5) nmol/l**		21.1	24.0
Serum B (74 ± 10)		81.8	71.6
Serum C (166 ± 16)		165	157

* Counts for Assay 1 mV · 20 s (integral), for Assay 2 mV/min (slope)

** Expression of the assay dynamic range

* Assays set up at the same time and measured manually on an LKB 1250 Luminometer (see l.c. (1) and (2))

** Target values ± 1 standard deviation – results are the mean of duplicate determinations.

Clinical examples of routine luminescence immunoassays – data from a caeruloplasmin SPALT, a C-reactive protein ILSA and a ferritin ILMA

Figures 4 and 5 show typical standard curves for caeruloplasmin and C-reactive protein respectively. The label for the caeruloplasmin SPALT was N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide, for C-reactive protein, diazoluminol. In both cases, the second antibody was labelled donkey anti-rabbit IgG. Table 11 shows clinical data obtained for different patient groups. The correlation between the ferritin assay here described and the radioimmunoassay used as its predecessor in the routine determination was excellent, ($n = 91$, $r = 0.992$, $a_{yx} = 0.071$ and $b_{yx} = 0.999$) when the same standards were used in each assay. Here the radioimmunoassay values were entered as x, those from the ILMA as y. The range of the values used for this calculation were 5–570 µg/l for the RIA and 3–567 µg/l for the ILMA.

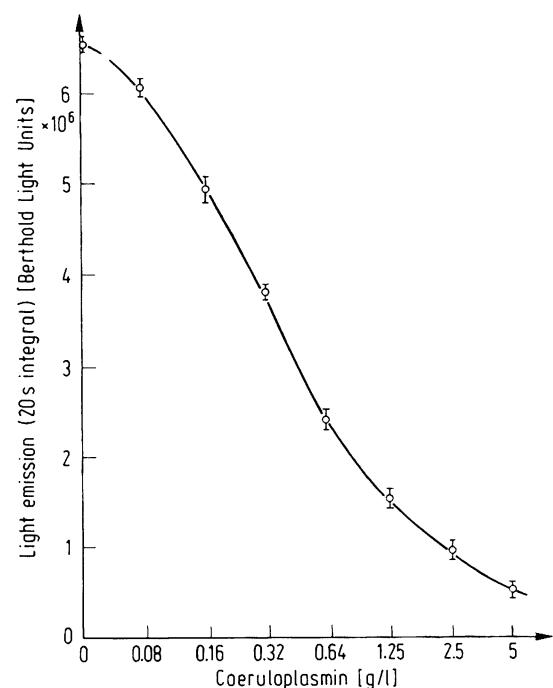


Fig. 4. Caeruloplasmin SPALT measured on the Berthold LB-950 luminometer. The ordinate represents the 20 s integral, expressed here in "Berthold light units" $\times 10^6$, as this luminometer employs photon counting techniques rather than the current amplification method used in the LKB instruments.

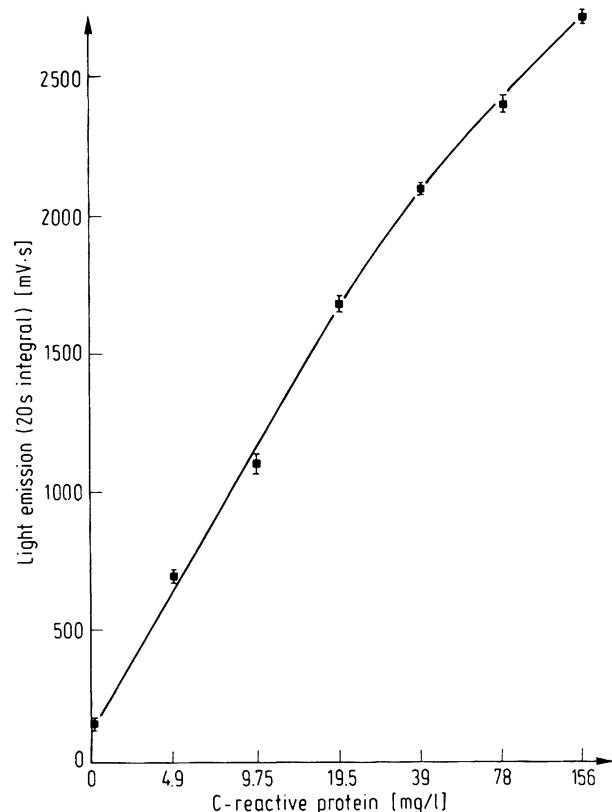


Fig. 5. C-reactive protein ILSA, using a diazoluminol labelled second antibody (donkey anti-rabbit IgG). This assay was measured on an LKB 1251 luminometer, the ordinate showing the 20 s integral value.

Tab. 11. Assay parameters and values from three experimental groups for caeruloplasmin, C-reactive protein and ferritin assays.

Parameter	Caerulo-plasmin	C-reactive protein	Ferritin
Assay type	SPALT	ILSA	ILMA
Label	ABEI-H ⁺	Diazoluminol	ABEI-H ⁺
Standard matrix	Buffer	Serum	Buffer
Standard	Human CP ⁺	Human CRP ⁺	Human LF ⁺
Reference range	0.15–0.65 g/l under 5 mg/l (serum)		30–300 µg/l
Assay working range ⁺⁺	0.15–1.25 g/l 2–160 mg/l		5–1000 µg/l
Mean precision (%) ⁺⁺⁺	5.8 (n = 205) 4.2 (n = 99)		4.3 (n = 1254)
Lower detection limit	<0.08 g/l <1 mg/l		<2 µg/l
Experimental groups			
<i>Crohn/Colitis</i>			
Range	0.14–0.53 g/l	1.72–60.2 mg/l	2–911 µg/l
Median	0.30 g/l	22.9 mg/l	23.8 µg/l
No. of elevated values*	0	18	4
No. of reduced values*	1	—	23
No. of patients in group	12	21	40
<i>Tumour bearers**</i>			
Range	0.13–2.34	0.8–139	3–2440
Median	0.44	11.8	152
No. of elevated values	12	14	14
No. of reduced values	1	—	4
No. of patients in group	35	18	42
<i>Blood donors – unselected</i>			
Range	0.06–1.01	0.5–10.7	5–240
Median	0.26	0.91	58
No. of elevated values	3	3	0
No. of reduced values	4	—	16
No. in group	45	64	84

* CP = caeruloplasmin, CRP = C-reactive protein, LF = liver ferritin, ABEI-H = N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide

** Range in which the mean precision is under 10%

+++ Actual precision within the working range – mean of all patients (n = . . .)

* Values lying below or above the established reference range.

** Pre-operative values – only patients with surgically confirmed tumours used in this analysis.

Discussion

The aim of this paper has been to put into practice some of the experiments performed in the first two parts of this series (1, 2). A comparison of both labels and methods has been made using a wide variety of antigens as ligands. Detailed clinical trials and evaluation results have been avoided, results being limited to a few assays, especially those shown in table 11.

The future of the luminescence immunoassay lies in its field of application, especially where its role as a practical alternative to routine radioimmunoassays is concerned. The assays presented here represent the whole gamut of molecular size and concentration found in in-vitro clinical chemistry and endocrinology.

The results of the comparison between a CELIA and ILMA using the same label and components (diazoluminol and immobilised sheep anti TBG) shows the relative sensitivity and working range of the two assay types, here for thyroxine binding globulin. The larger working range of the ILMA agrees with the findings of Hunter (6) who compared radioimmunoassays and immunoradiometric assays for sensitivity and working range. The TBG CELIA, although giving a dose response curve when the standards were dissolved in a buffer matrix, was unable to be used for measuring serum samples, where all values lay above the highest standard. The combination of the relatively large sample volume (50 µl) and contact between serum and label may be a crucial factor with the CELIA, as the TBG ILMA, where a much smaller sample (1 µl) was used, and where serum and label did not come into contact, measured correctly. Similar problems were encountered with a thyroxine CELIA using larger serum volumes (50 µl) and low-titer low affinity antibodies (Gadow, unpublished results).

The comparison between the different labels is well demonstrated in the case of the ferritin assays (table 7, figure 2). Although the detection limits of free diazoluminol and N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide were similar (2), the N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide label allowed an assay to be developed which was sensitive enough for routine use. This was probably due to the difference in the chemical coupling methods used, the N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide active ester being under neutral and mild reaction conditions, the diazo coupling taking place in alkaline solution over a period of several hours. The ferritin assays show the relative performance of ILMA and ILSA using the same label (here diazolu-

minol). The dynamic range of the N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide labelled ferritin ILMA is far greater than that using diazoluminol as label. This is reflected in the ratio between the number of counts in the highest standard and those in the zero standard, (see tab. 7). This ratio was 54:1 for N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide labelled anti ferritin and only 4.9:1 for diazoluminol labelled anti ferritin.

Various conditions have been described for the optimal conditions for light emission which range from initiation at pH 8–9 (7) via pH 13 (4) to initiation after standing in alkaline solution for several minutes (8) to a few hours (Kohen, personal communication). The cortisol SPALT (see tab. 8 and 9) was used to compare the effect of pH and alkaline incubation on the light output. Although the signal increases between pH 8 and pH 13 as well as between pH 13 when measured immediately and after 2 h standing in sodium hydroxide, the signal to noise ratio, expressed in terms of the zero standard (B_0) and unspecific binding (UB) increased only slightly.

The dynamic range of the assay, expressed as the light signal given by the zero standard and that given by the highest standard, remained almost unchanged between pH 8 and pH 13, and was noticeably reduced after prolonged alkaline incubation before light initiation.

The values of the control sera lay within the expected limits for all assays.

The thyroxine SPALT was used to demonstrate the use of bioluminescent and chemiluminescent labels. The bioluminescent SPALT had a larger dynamic range when compared with the diazoluminol labelled assay, and was potentially more sensitive, as can be seen from the intercept values (tab. 10). Both assays measured correctly in terms of the control sera. Replacement of the diazoluminol labelled second antibody by one labelled with N-(4-aminobutyl)-N-ethyl

isoluminol hemisuccinamide gave rise to a similar increase in the dynamic range as seen in the ferritin ILMA, so that for the routine assay, N-(4-aminobutyl)-N-ethyl isoluminol hemisuccinamide was chosen as label.

As stated above, the proof of the assays is in their clinical routine application and examples have been presented for ferritin, C-reactive protein and caeruloplasmin, all of which are the only routine assay for these components. The results shown are taken from projects on patients with tumours and with *Crohn's* disease or ulcerative colitis (see tab. 11). The screening of blood donors is part of an ongoing routine procedure, especially upon new and regular donors.

The mean precision within the working range, here derived from compound precision profiles, was acceptable and comparable with commercial tests. A further advantage of these tests was their suitability for paediatric use, the largest sample volume being 20 µl for ferritin.

One thing became clear when working with immobilised antibodies, and that was the necessity for partial purification of the native antisera before coupling to the solid phase. This was effected by precipitation of the γ-globulin fraction with 200 g/l polyethylene glycol (M_r 6000) with resolution of the precipitate in 0.02 mol/l phosphate buffer, pH 8. Subsequent passage over a DEAE-cellulose column was sufficient to give a product with acceptable purity.

To conclude, it has been shown that the application of luminescence immunoassays in routine in-vitro diagnosis is now possible, although the acceptance of such assays still depends upon the commercialisation of the methods.

Acknowledgements

The authors wish to thank Frau Jutta Jäger for technical assistance.

References

1. Wood, W. G. & Gadow, A. (1983) *J. Clin. Chem. Clin. Biochem.* **21**, 789–797.
2. Gadow, A., Fricke, H. & Wood, W. G. (1984) *J. Clin. Chem. Clin. Biochem.* **22**, 337–347.
3. Miles, L. E. M. & Hales, C. N. (1968) *Nature* **219**, 186.
4. Strasburger, C. J., Fricke, H. & Wood, W. G. (1982) In: *Radioimmunoassay and related procedures in medicine 1982*, IAEA, Vienna, pp. 757–777.
5. Wood, W. G., Fricke, H., von Klitzing, L., Strasburger, C. J. & Scriba, P. C. (1982) *J. Clin. Chem. Clin. Biochem.* **20**, 825–831.
6. Hunter, W. M. (1982) In: *Radioimmunoassay and related procedure in medicine 1982*, IAEA, Vienna, pp. 3–21.
7. Kohen, F., Kim, J. B. & Lindner, H. R. (1981) In: *Bioluminescence and chemiluminescence, basic chemistry and analytical applications* (DeLuca, Marlene A., McElroy, W. D., eds.) Academic Press, New York, pp. 357–364.
8. Strasburger, C. J., Fricke, H. & Wood, W. G. (1982) *Fresenius Z. Anal. Chem.* **311**, 351–352.

Priv.-Doz. Dr. W. G. Wood
Klinische Laboratorien
Klinik für Innere Medizin
Medizinische Hochschule Lübeck
Ratzeburger Allee 160
D-2400 Lübeck 1